

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022159.D
 Acq On : 03 Mar 2022 13:22
 Operator : SY/VA
 Sample : N1733-04
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 04 00:32:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	196886	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	178224	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	89202	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	40131	15.627	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	62.520%		
7) Chloroethane-d5	2.879	69	32826	16.246	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	65.000%		
11) 1,1-Dichloroethene-d2	4.013	63	51034	12.977	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	51.920%		
21) 2-Butanone-d5	7.074	46	23875	55.295	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.600%		
24) Chloroform-d	7.647	84	98560	22.437	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.760%		
26) 1,2-Dichloroethane-d4	8.305	65	52377	22.938	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.760%		
32) Benzene-d6	8.275	84	181463	21.877	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.520%		
36) 1,2-Dichloropropane-d6	9.275	67	53936	23.415	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.680%		
41) Toluene-d8	10.323	98	175181	21.244	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.960%		
43) trans-1,3-Dichloroprop...	10.579	79	21276	20.832	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.320%		
47) 2-Hexanone-d5	10.927	63	19991	52.767	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.540%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	49657	24.564	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.240%		
66) 1,2-Dichlorobenzene-d4	13.853	152	68050	23.751	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	95.000%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	9.275	63	6612	3.289	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022159.D
Acq On : 03 Mar 2022 13:22
Operator : SY/VA
Sample : N1733-04
Misc : 6.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 04 00:32:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

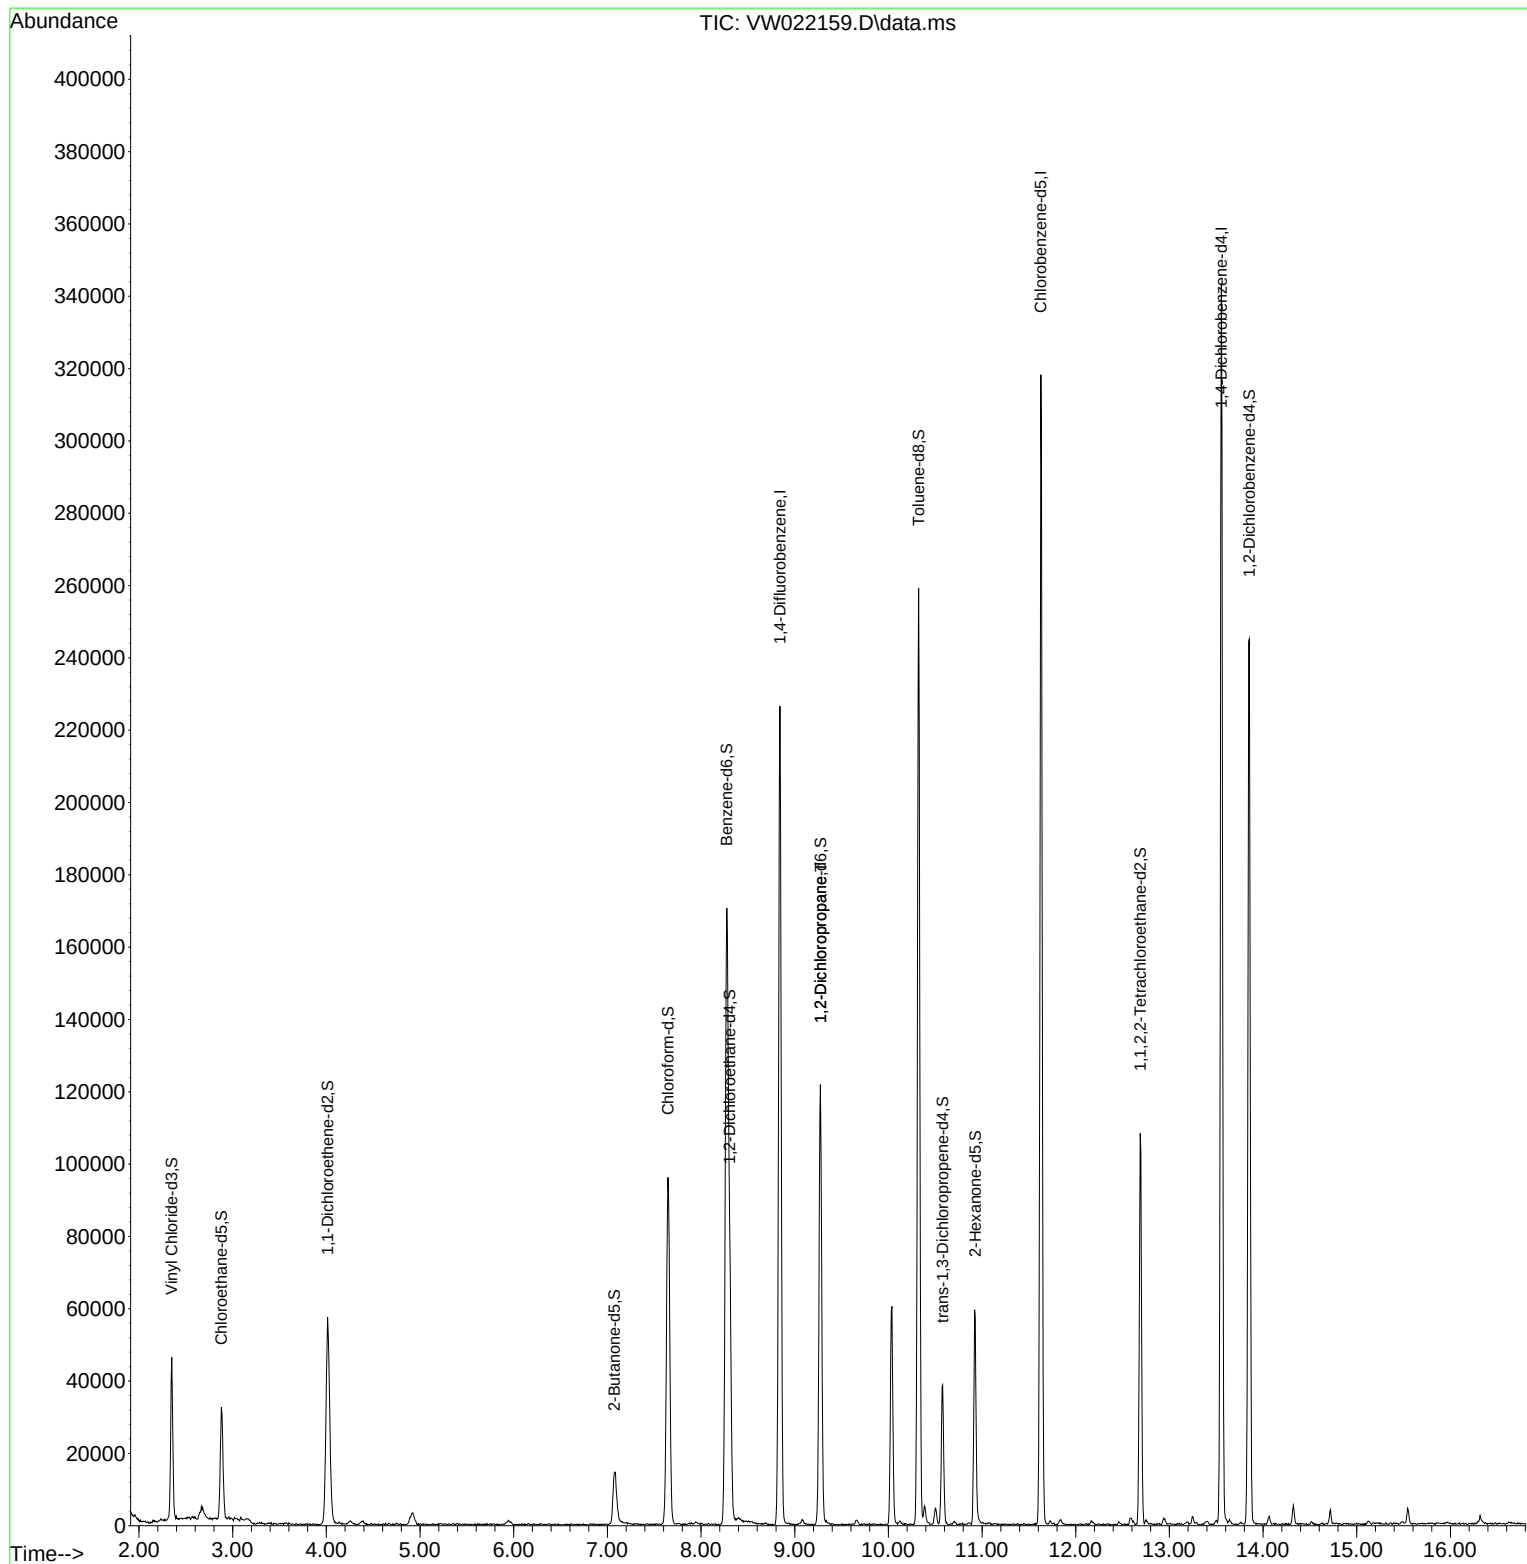

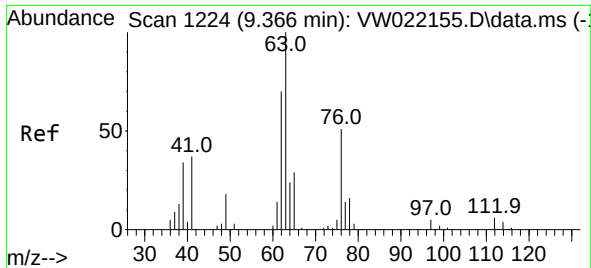

#37

1,2-Dichloropropane

Concen: 3.289 ug/L

RT: 9.275 min Scan# 11

Delta R.T. -0.091 min


Lab File: VW022159.D

Acq: 03 Mar 2022 13:22

Instrument :

MSVOA_W

ClientSampleId :

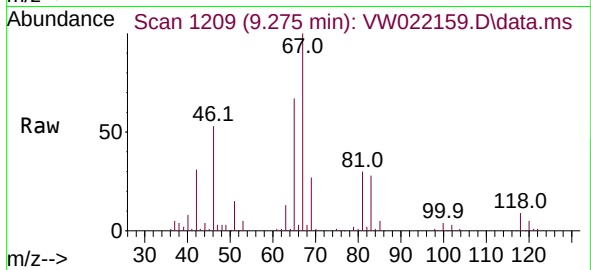

Tgt Ion: 63 Resp: 6612

Ion	Ratio	Lower	Upper
63	100		
112	0.0	4.1	6.1#

