




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022160.D
 Acq On : 03 Mar 2022 13:46
 Operator : SY/VA
 Sample : N1733-05
 Misc : 6.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRR9

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:32:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

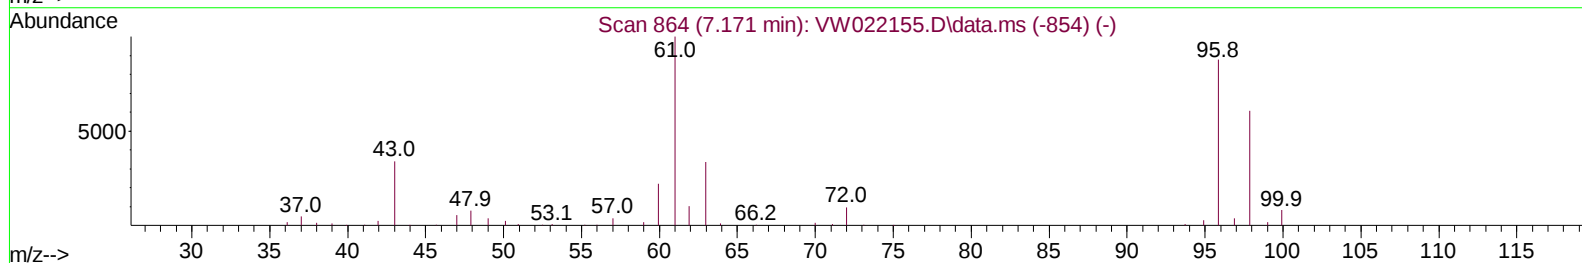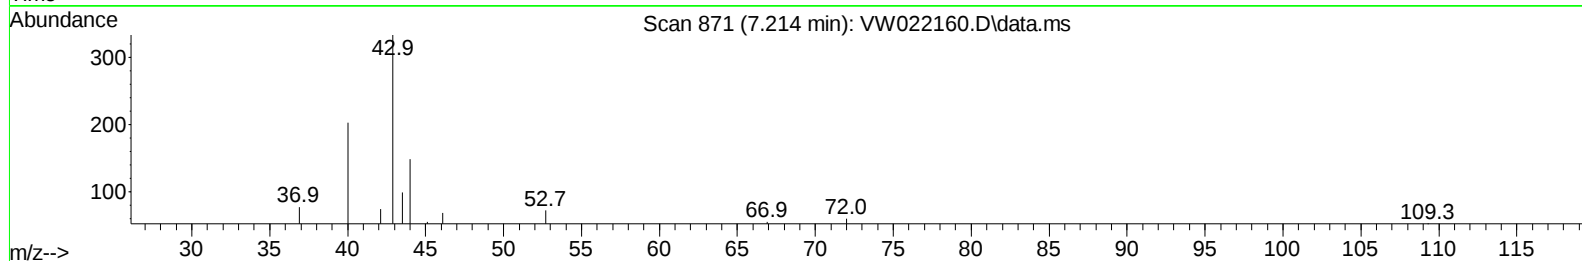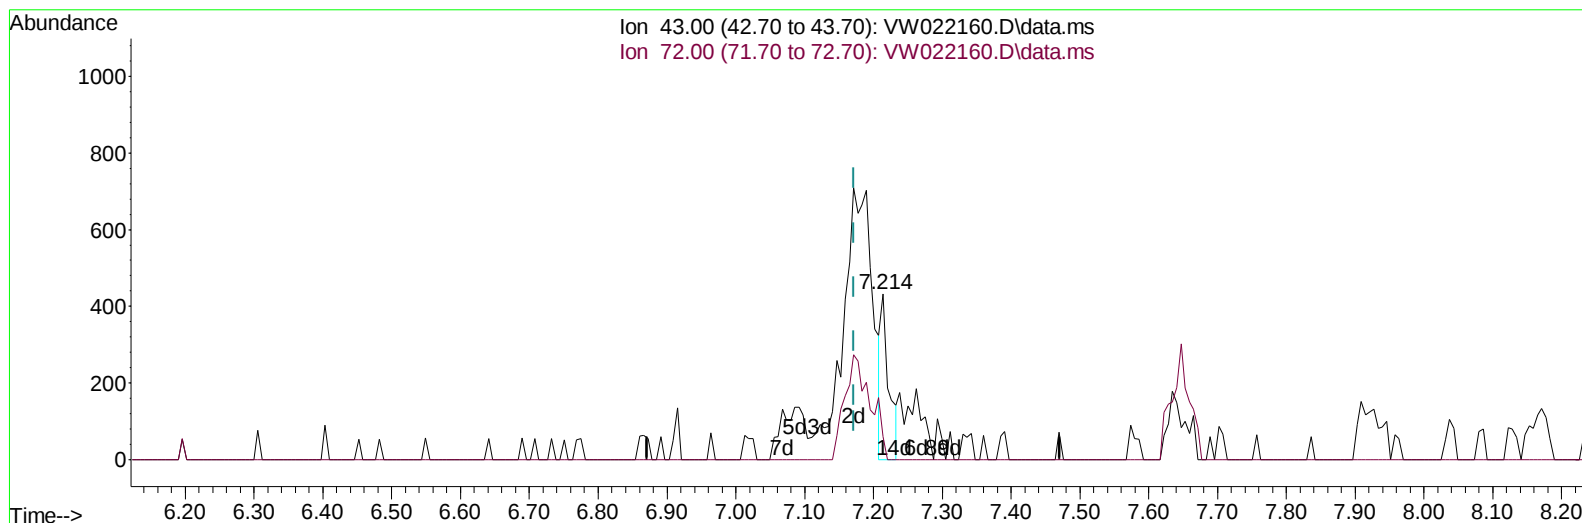

TIC: VW022160.D\data.ms

(22) 2-Butanone (T)

7.214min (+ 0.043) 0.90 ug/L

response 335

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	34.00	24.18
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022160.D
 Acq On : 03 Mar 2022 13:46
 Operator : SY/VA
 Sample : N1733-05
 Misc : 6.97g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRR9

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:32:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

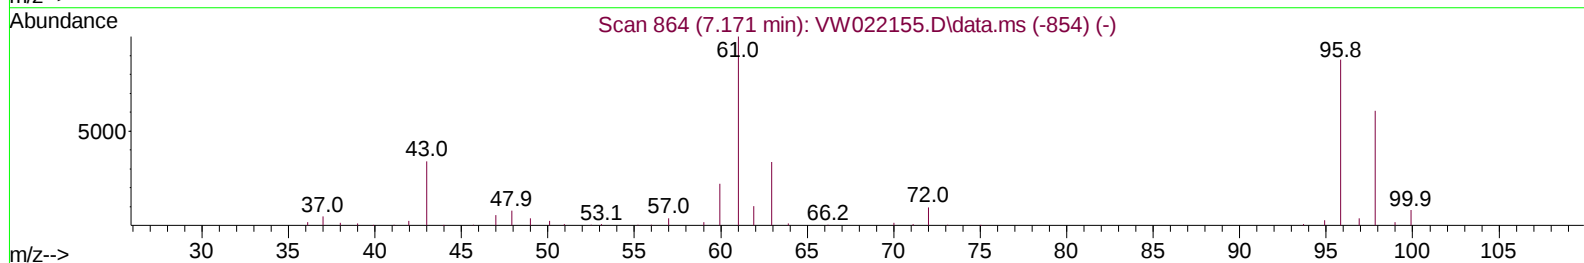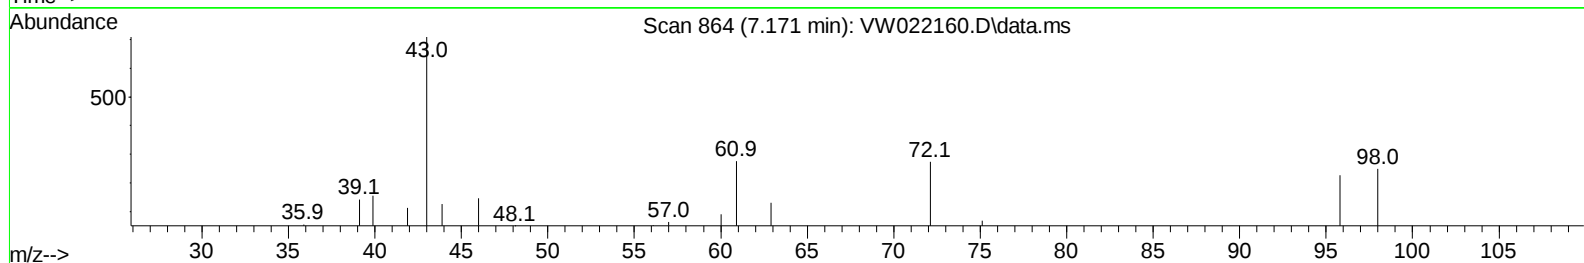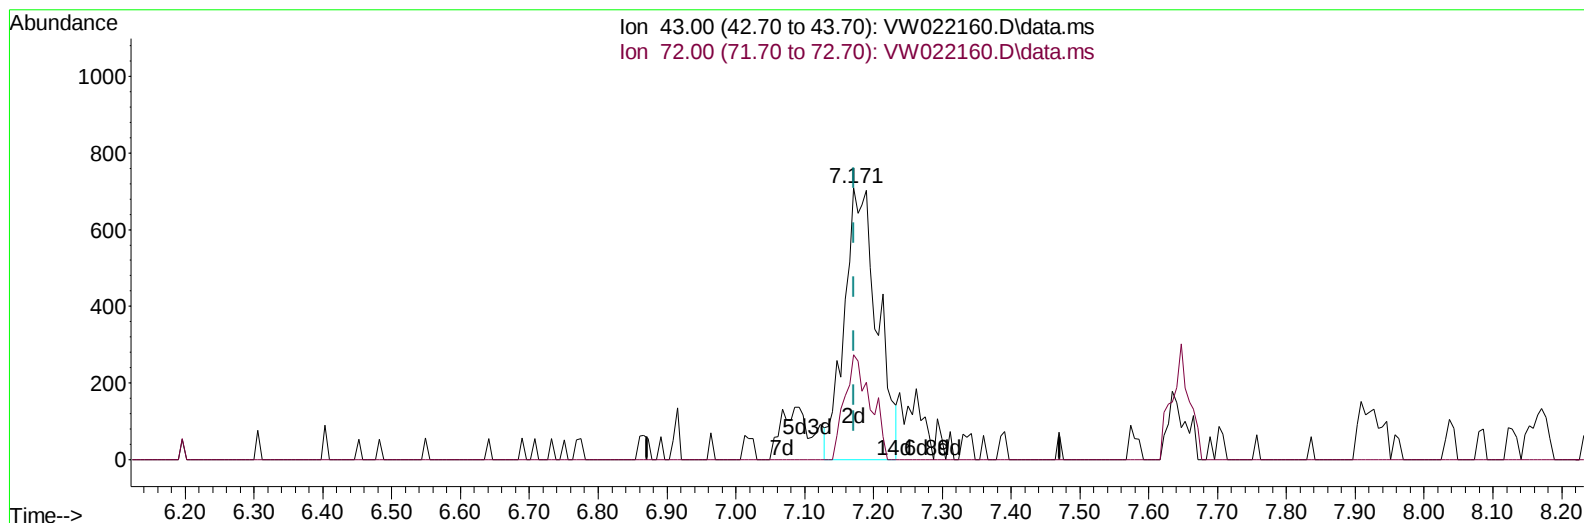

TIC: VW022160.D\data.ms

(22) 2-Butanone (T)

7.171min (+ 0.000) 6.31 ug/L m

response 2349

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	34.00	3.45#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022160.D
 Acq On : 03 Mar 2022 13:46
 Operator : SY/VA
 Sample : N1733-05
 Misc : 6.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRR9

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:32:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	144633	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	134574	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	69983	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	29128	15.441	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	61.760%	
7) Chloroethane-d5	2.879	69	23717	15.979	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.920%	
11) 1,1-Dichloroethene-d2	4.013	63	36627	12.679	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	50.720%	
21) 2-Butanone-d5	7.074	46	25794	81.323	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	162.640%#	
24) Chloroform-d	7.647	84	71363	22.115	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.440%	
26) 1,2-Dichloroethane-d4	8.305	65	41870	24.961	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	99.840%	
32) Benzene-d6	8.275	84	131428	20.985	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.920%	
36) 1,2-Dichloropropane-d6	9.274	67	40278	23.157	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	92.640%	
41) Toluene-d8	10.323	98	123282	19.799	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.200%	
43) trans-1,3-Dichloroprop...	10.579	79	16699	21.653	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	86.600%	
47) 2-Hexanone-d5	10.921	63	21421	74.881	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	149.760%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	47784	31.304	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	125.200%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	53666	23.875	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	95.520%	
Target Compounds						
13) Acetone	4.141	43	1127	4.350	ug/L	63
22) 2-Butanone	7.171	43	2349m	6.312	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022160.D
Acq On : 03 Mar 2022 13:46
Operator : SY/VA
Sample : N1733-05
Misc : 6.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRR9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:32:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

