




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022165.D
 Acq On : 03 Mar 2022 15:48
 Operator : SY/VA
 Sample : N1733-07
 Misc : 5.28g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS2

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

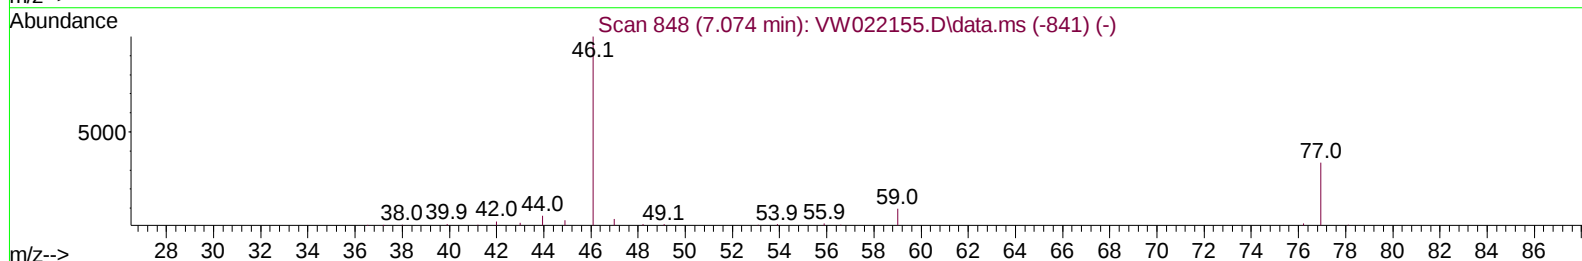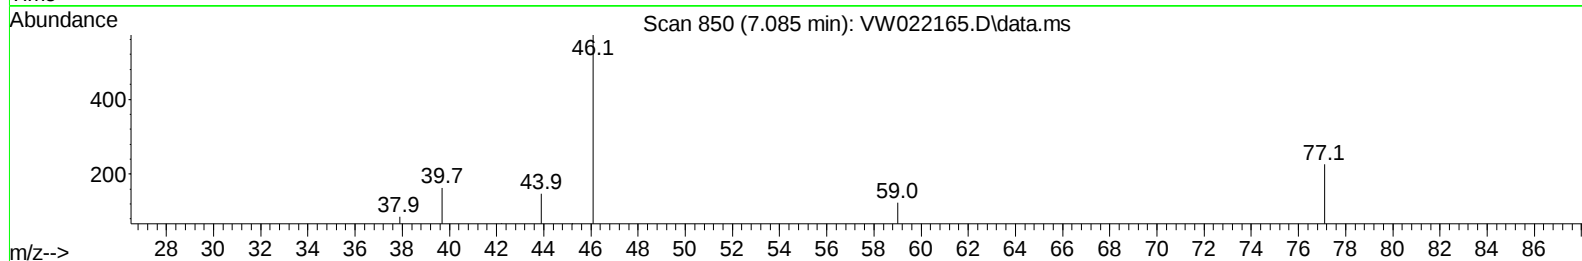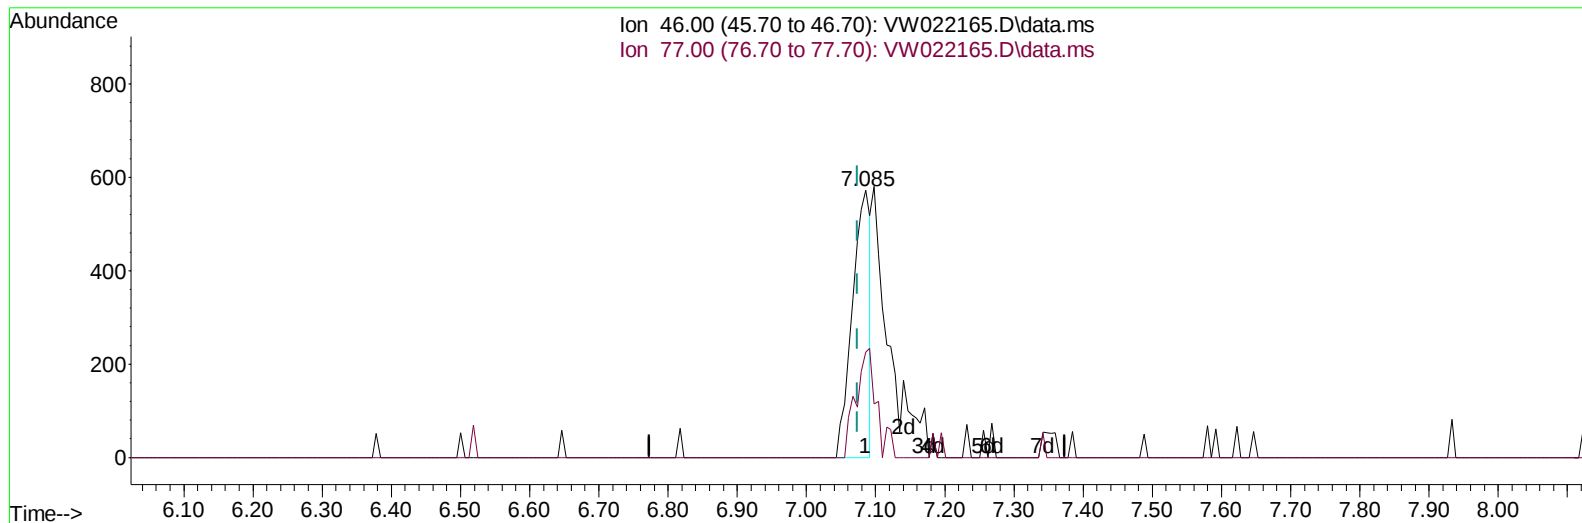

TIC: VW022165.D\data.ms

(21) 2-Butanone-d5 (S)

7.085min (+ 0.012) 42.60 ug/L

response 1037

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	28.10	31.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022165.D
Acq On : 03 Mar 2022 15:48
Operator : SY/VA
Sample : N1733-07
Misc : 5.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:34:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

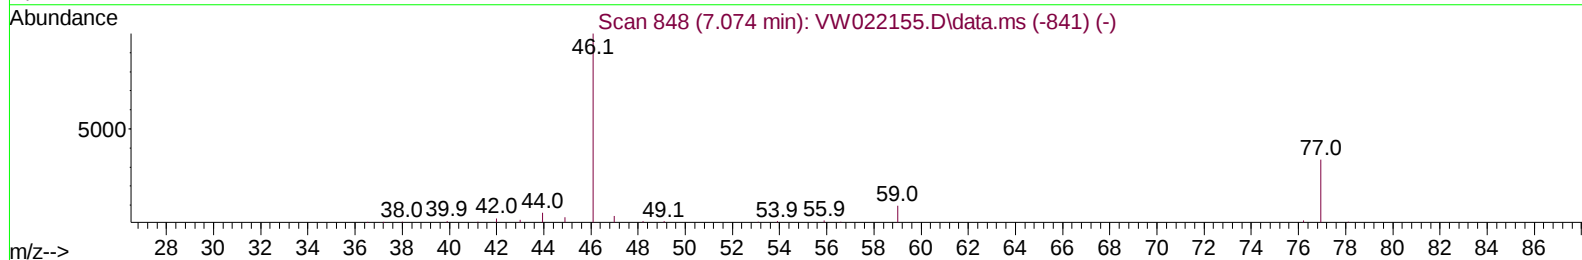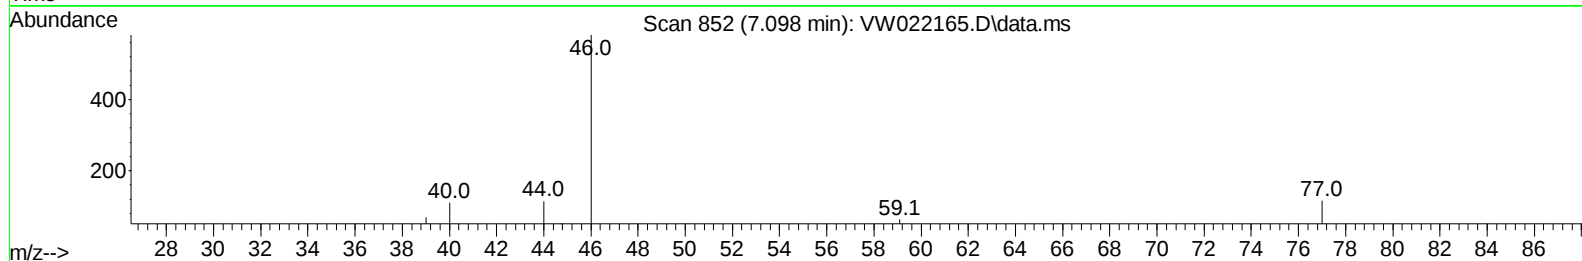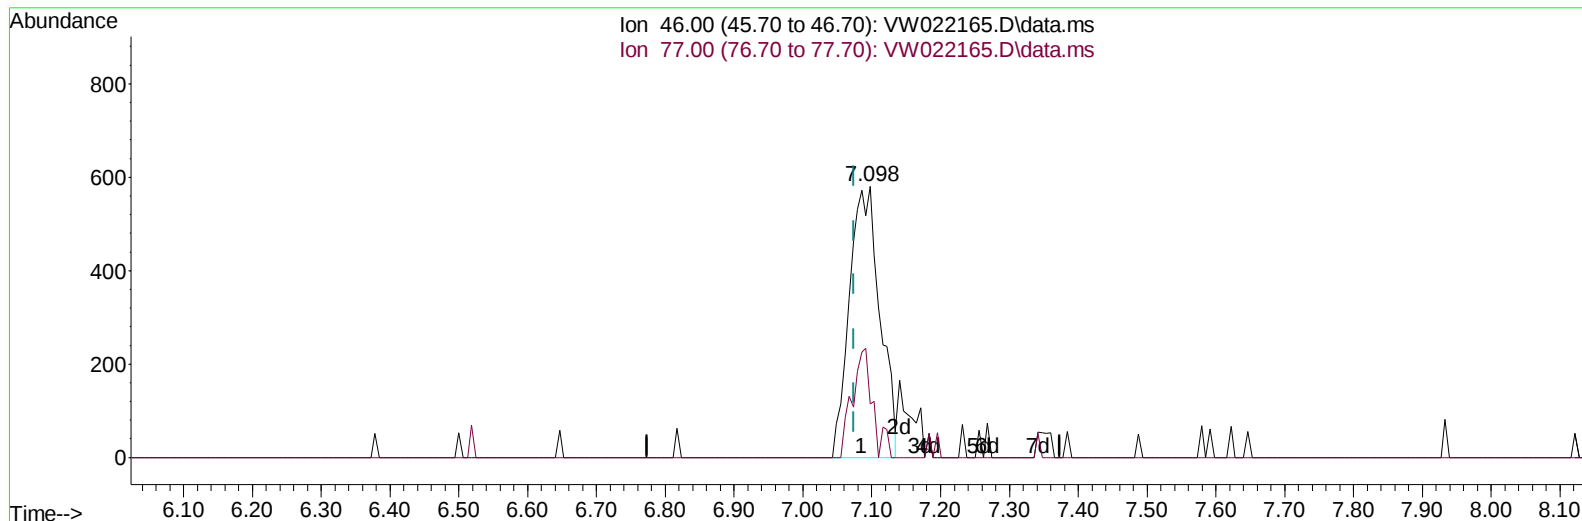

TIC: VW022165.D\data.ms

(21) 2-Butanone-d5 (S)

7.098min (+ 0.024) 73.38 ug/L m

response 1786

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	28.10	18.03#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022165.D
 Acq On : 03 Mar 2022 15:48
 Operator : SY/VA
 Sample : N1733-07
 Misc : 5.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS2

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	11099	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	9918	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	4221	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	2888	19.950	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	79.800%		
7) Chloroethane-d5	2.891	69	2259	19.833	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	79.320%		
11) 1,1-Dichloroethene-d2	4.025	63	4198	18.936	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	75.760%		
21) 2-Butanone-d5	7.098	46	1786m	73.377	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery =	146.760%#		
24) Chloroform-d	7.652	84	6695	27.036	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	108.160%		
26) 1,2-Dichloroethane-d4	8.305	65	3664	28.464	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	113.840%		
32) Benzene-d6	8.280	84	11696	25.339	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	101.360%		
36) 1,2-Dichloropropane-d6	9.274	67	3619	28.232	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	112.920%		
41) Toluene-d8	10.323	98	10061	21.924	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	87.680%		
43) trans-1,3-Dichloroprop...	10.579	79	1241	21.835	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	87.320%		
47) 2-Hexanone-d5	10.926	63	1012	48.001	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	96.000%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	3227	28.685	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	114.720%		
66) 1,2-Dichlorobenzene-d4	13.846	152	3713	27.387	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	109.560%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022165.D
Acq On : 03 Mar 2022 15:48
Operator : SY/VA
Sample : N1733-07
Misc : 5.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:34:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

