




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022166.D
 Acq On : 03 Mar 2022 16:12
 Operator : SY/VA
 Sample : N1733-08
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS3

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

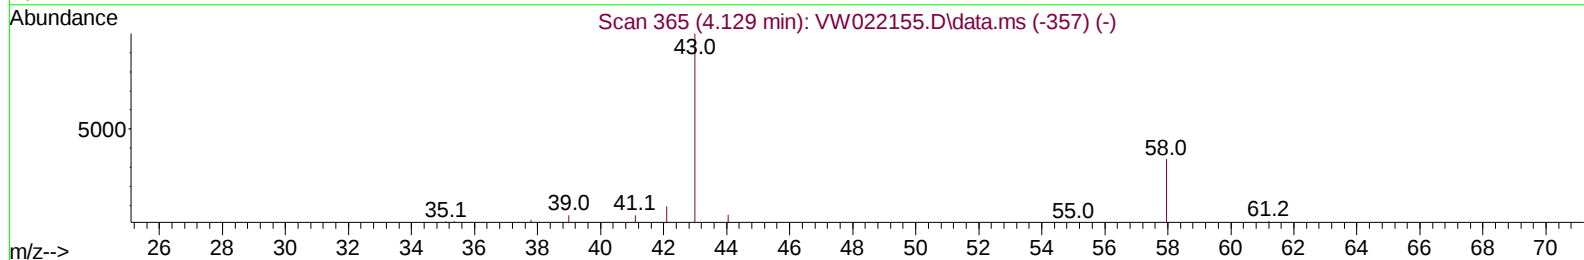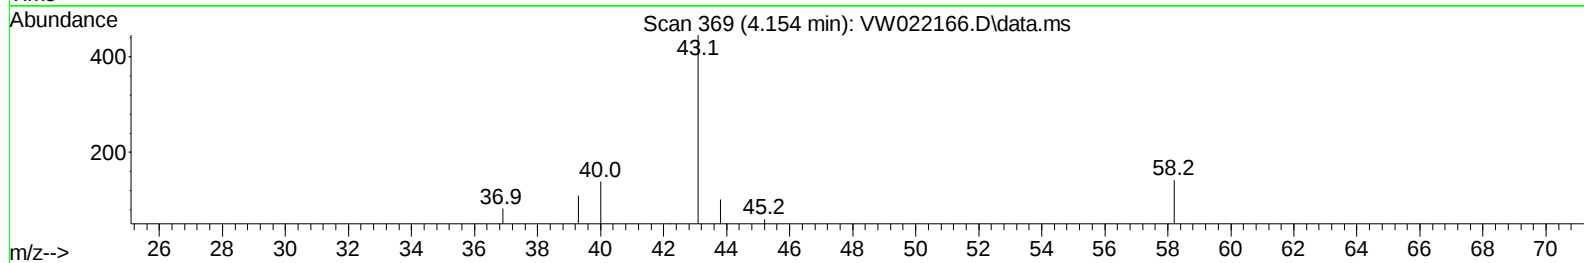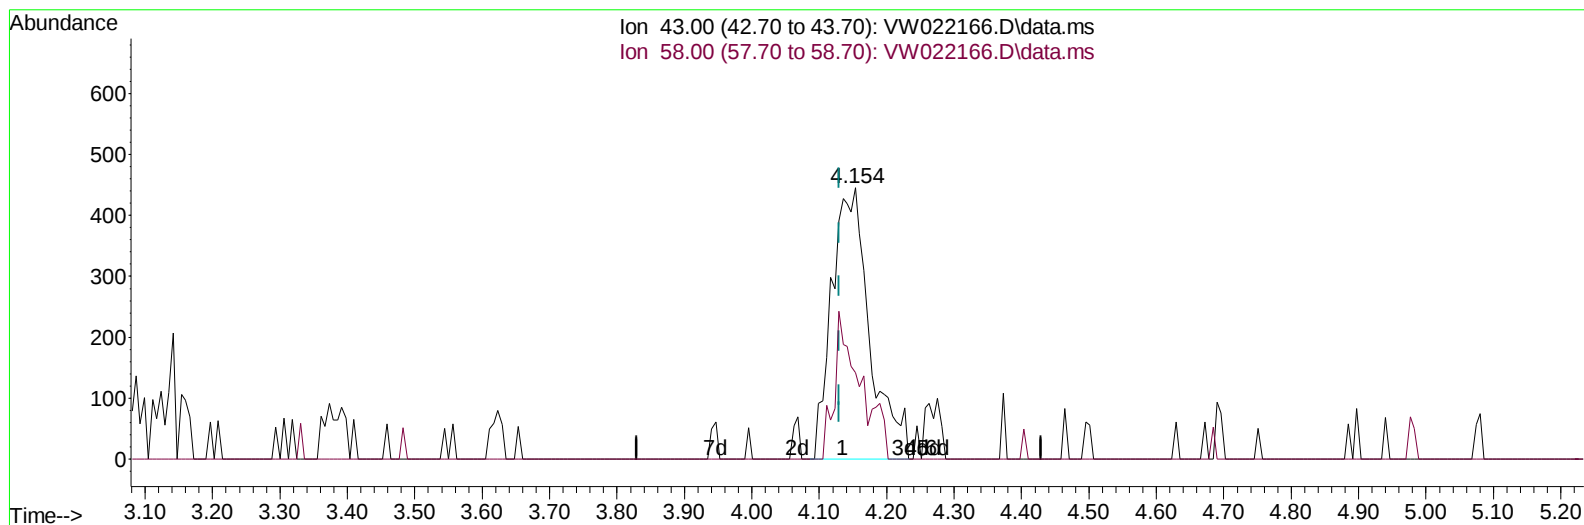

TIC: VW022166.D\data.ms

(13) Acetone (T)

4.154min (+ 0.025) 7.25 ug/L m

response 1741

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	23.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022166.D
 Acq On : 03 Mar 2022 16:12
 Operator : SY/VA
 Sample : N1733-08
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS3

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	134027	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	126245	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	60898	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	31114	17.798	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.200%	
7) Chloroethane-d5	2.879	69	26659	19.382	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.520%	
11) 1,1-Dichloroethene-d2	4.013	63	37665	14.070	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.280%	
21) 2-Butanone-d5	7.080	46	17764	60.438	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.880%	
24) Chloroform-d	7.647	84	69995	23.407	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	93.640%	
26) 1,2-Dichloroethane-d4	8.305	65	37611	24.196	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	96.800%	
32) Benzene-d6	8.275	84	128381	21.850	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	87.400%	
36) 1,2-Dichloropropane-d6	9.275	67	38630	23.675	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	94.720%	
41) Toluene-d8	10.323	98	121370	20.778	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	83.120%	
43) trans-1,3-Dichloroprop...	10.573	79	14664	20.269	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	81.080%	
47) 2-Hexanone-d5	10.921	63	15007	55.920	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	111.840%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	36008	25.146	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	100.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152	51261	26.207	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	104.840%	
Target Compounds						
13) Acetone	4.154	43	1741m	7.252	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022166.D
Acq On : 03 Mar 2022 16:12
Operator : SY/VA
Sample : N1733-08
Misc : 4.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:34:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

