




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022167.D
 Acq On : 03 Mar 2022 16:36
 Operator : SY/VA
 Sample : N1733-09
 Misc : 11.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS4

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

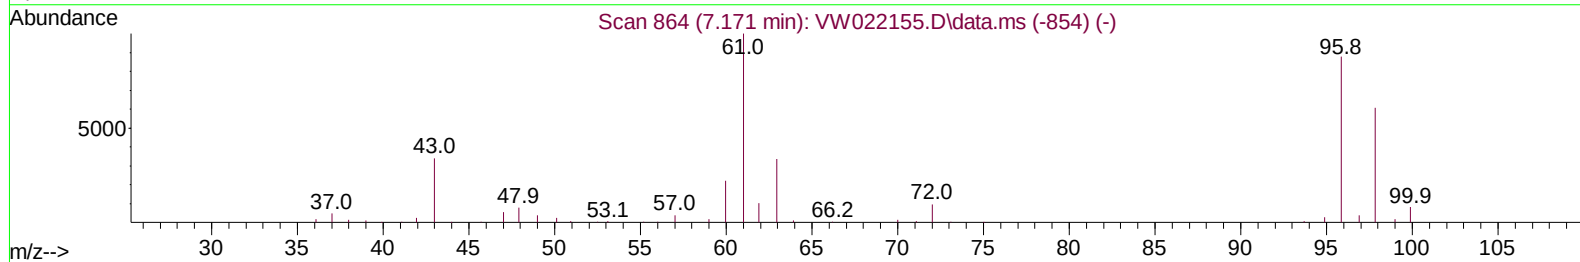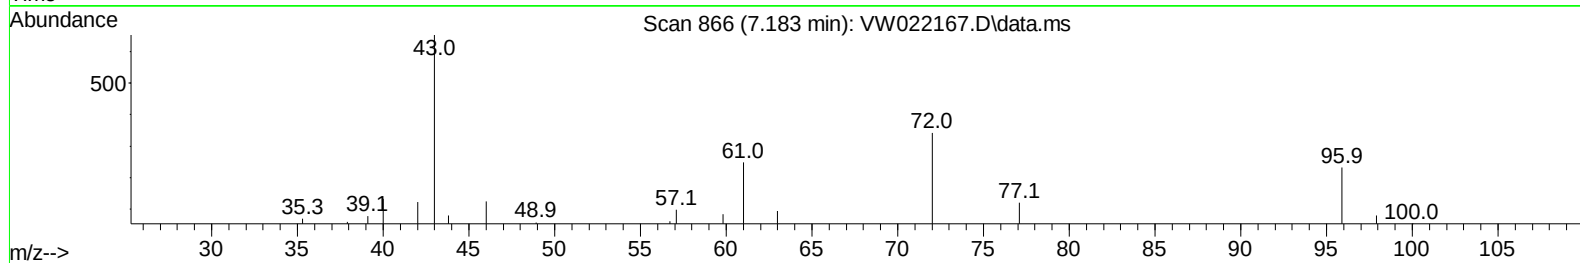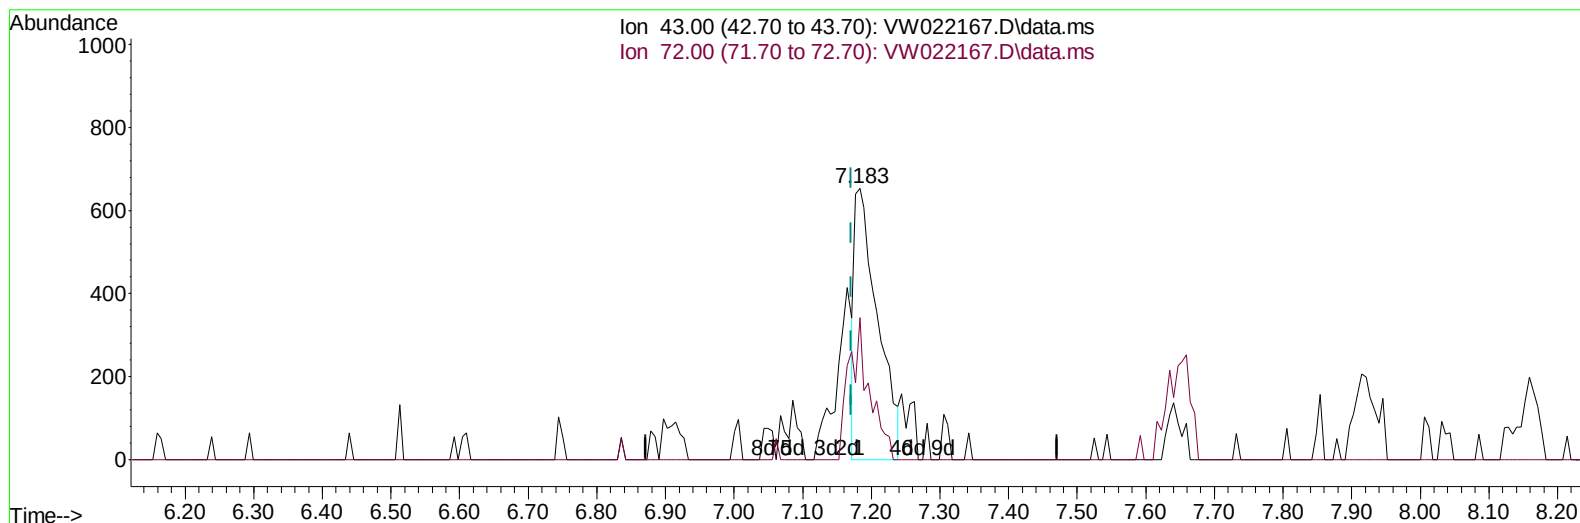

TIC: VW022167.D\data.ms

(22) 2-Butanone (T)

7.183min (+ 0.012) 4.10 ug/L

response 1523

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	34.00	27.31
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022167.D
 Acq On : 03 Mar 2022 16:36
 Operator : SY/VA
 Sample : N1733-09
 Misc : 11.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS4

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

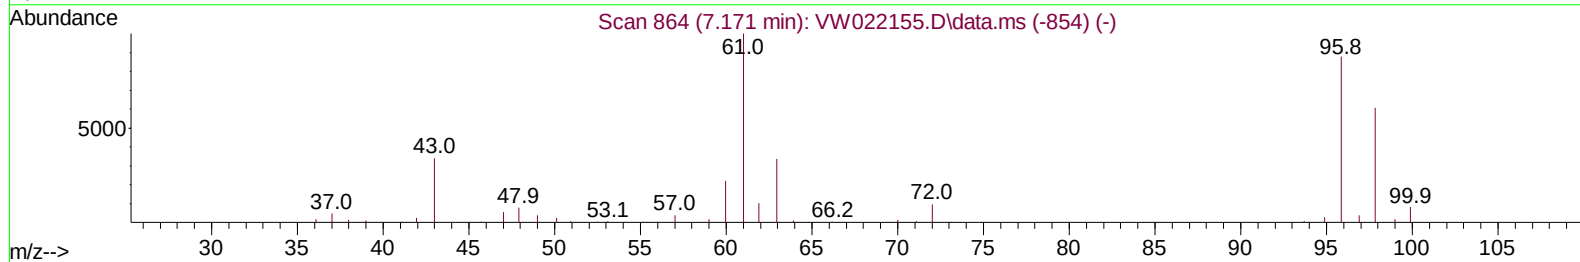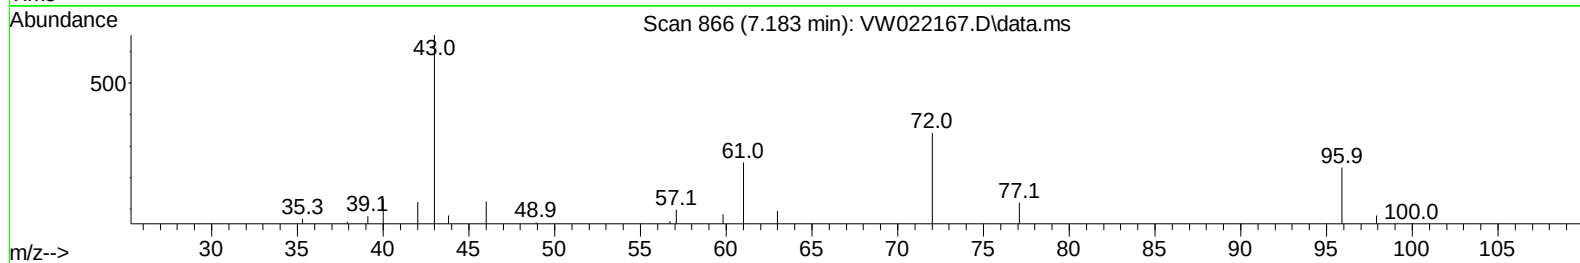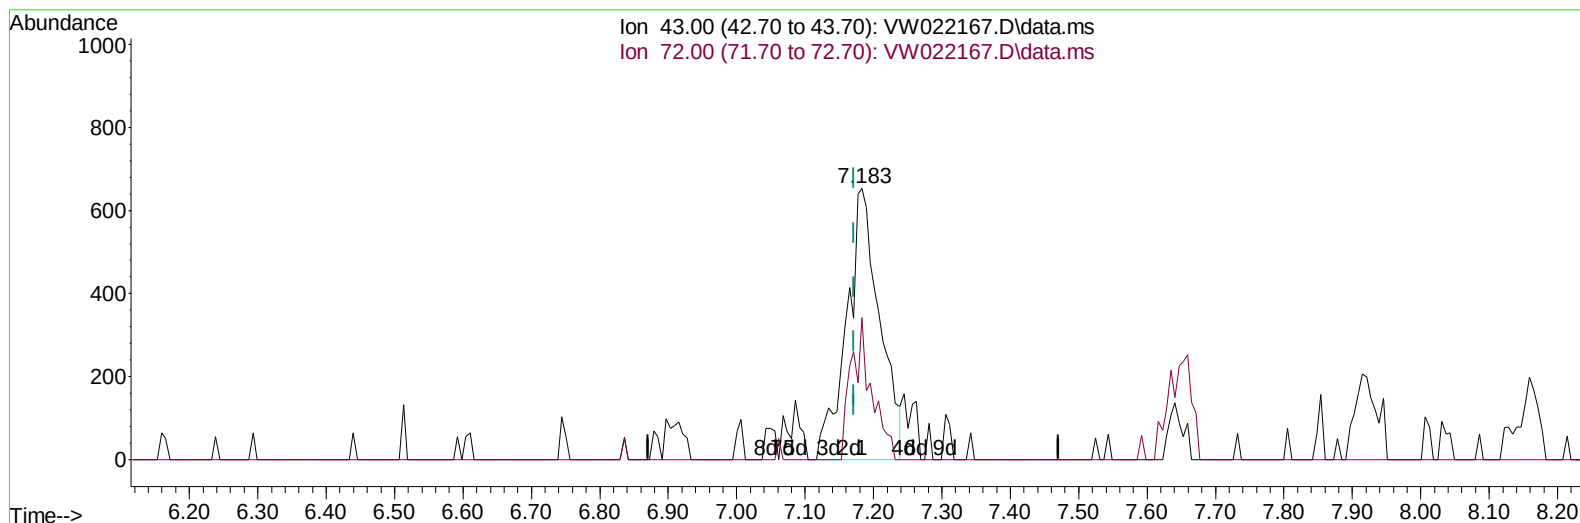

TIC: VW022167.D\data.ms

(22) 2-Butanone (T)

7.183min (+ 0.012) 5.88 ug/L m

response 2187

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	34.00	19.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022167.D
 Acq On : 03 Mar 2022 16:36
 Operator : SY/VA
 Sample : N1733-09
 Misc : 11.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:34:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		144482	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		138705	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		72354	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		28955	15.365	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	61.440%		
7) Chloroethane-d5	2.885	69		24028	16.205	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.840%		
11) 1,1-Dichloroethene-d2	4.013	63		35525	12.310	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	49.240%		
21) 2-Butanone-d5	7.086	46		21049	66.432	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135		Recovery =	132.860%		
24) Chloroform-d	7.647	84		70202	21.778	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	87.120%		
26) 1,2-Dichloroethane-d4	8.305	65		39235	23.415	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	93.640%		
32) Benzene-d6	8.275	84		126561	19.606	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	78.440%		
36) 1,2-Dichloropropane-d6	9.268	67		39600	22.089	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	88.360%		
41) Toluene-d8	10.323	98		120560	18.785	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	75.160%		
43) trans-1,3-Dichloroprop...	10.579	79		16041	20.181	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	80.720%		
47) 2-Hexanone-d5	10.921	63		18417	62.462	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	124.920%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		42335	26.908	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	107.640%		
66) 1,2-Dichlorobenzene-d4	13.847	152		54454	23.432	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	93.720%		
Target Compounds							
13) Acetone	4.141	43		3510	13.563	ug/L	51
22) 2-Butanone	7.183	43		2187m	5.883	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022167.D
Acq On : 03 Mar 2022 16:36
Operator : SY/VA
Sample : N1733-09
Misc : 11.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:34:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

