




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022168.D
 Acq On : 03 Mar 2022 17:00
 Operator : SY/VA
 Sample : N1733-13
 Misc : 6.66g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS6

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

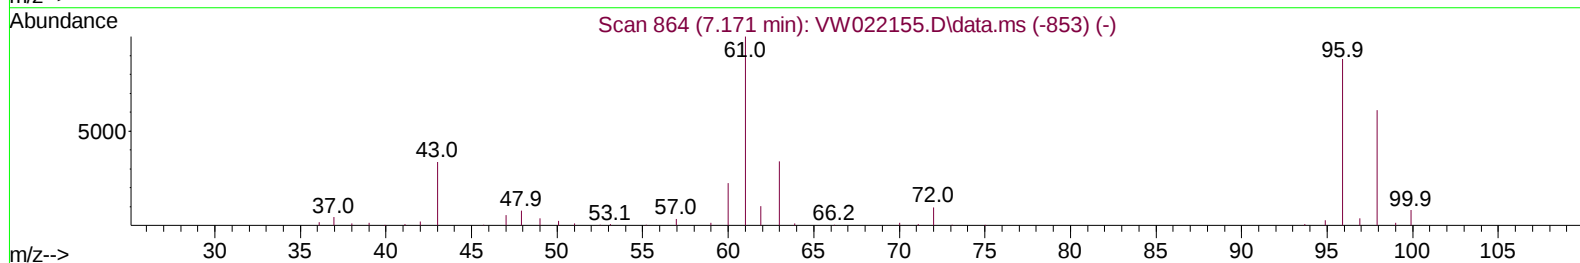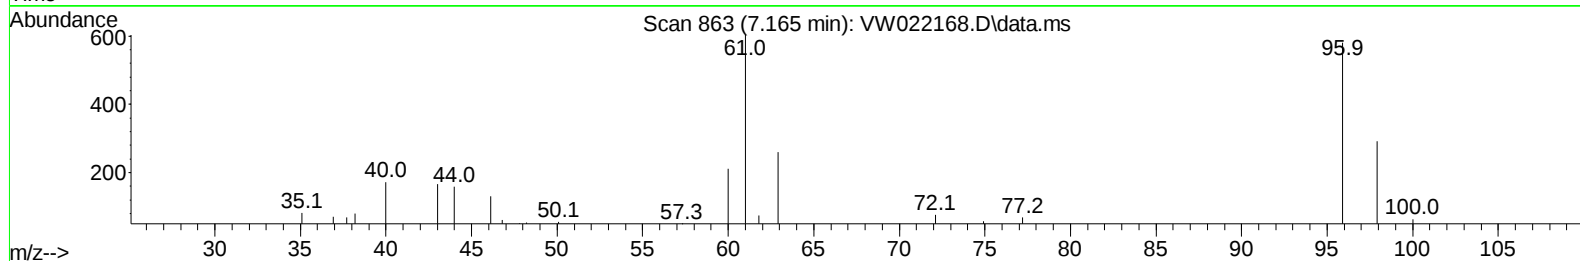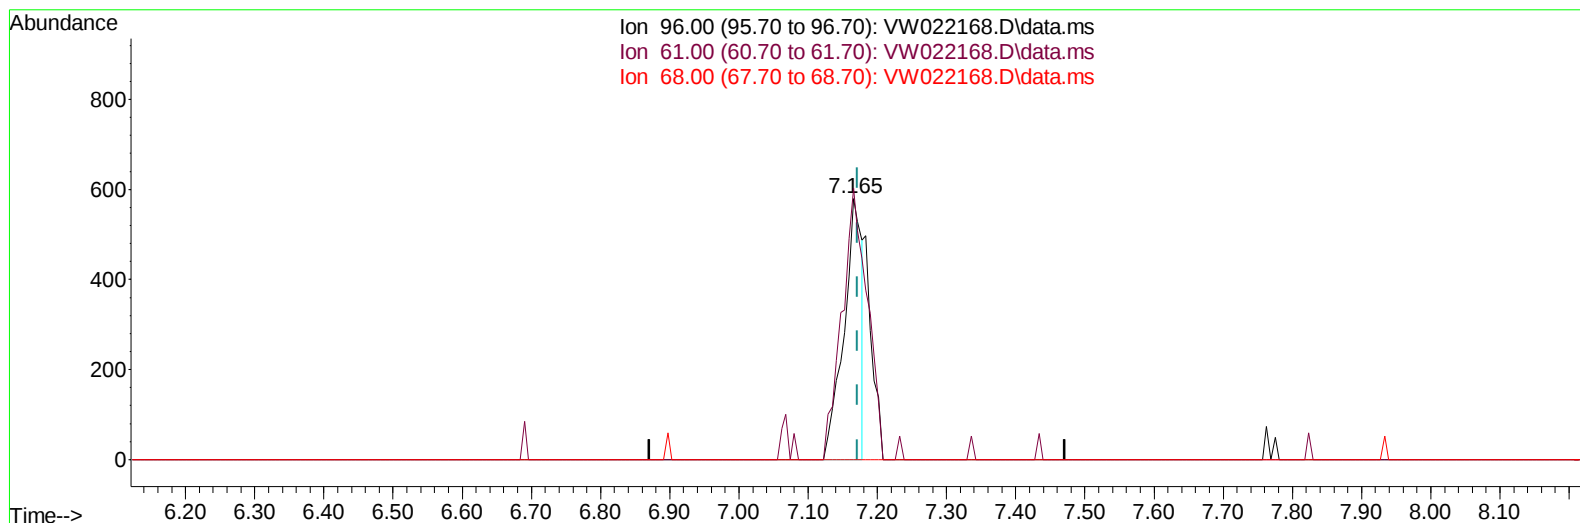

TIC: VW022168.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.165min (-0.006) 0.49 ug/L

response 1040

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	109.70	103.97
68.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022168.D
Acq On : 03 Mar 2022 17:00
Operator : SY/VA
Sample : N1733-13
Misc : 6.66g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS6

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

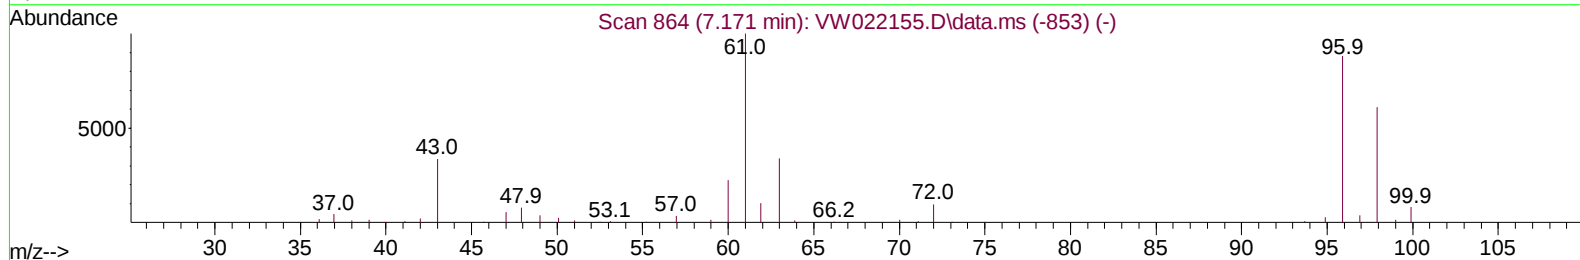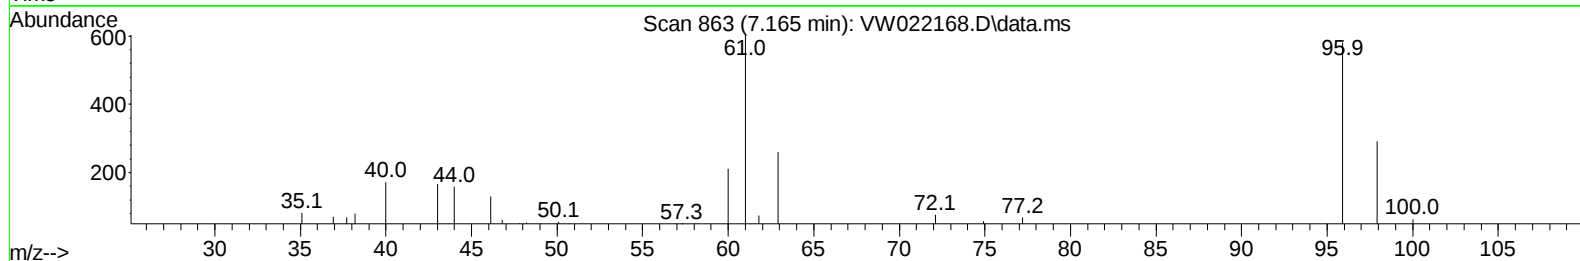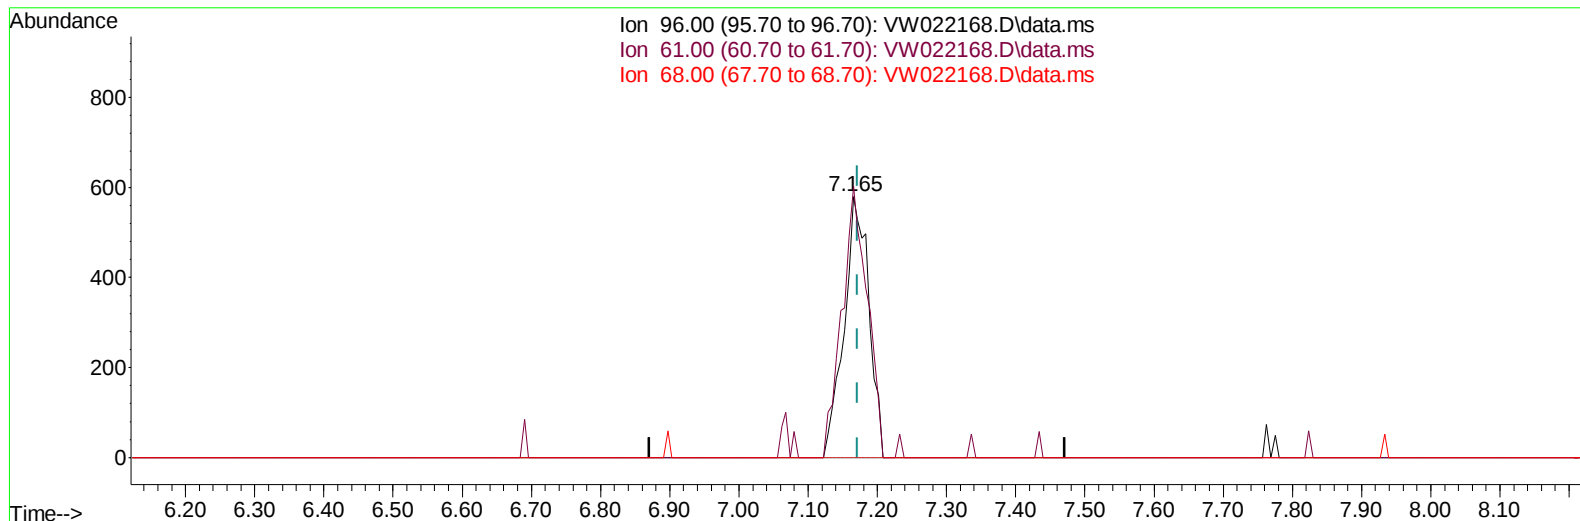

TIC: VW022168.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.165min (-0.006) 0.69 ug/L m

response 1441

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	109.70	103.97
68.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022168.D
 Acq On : 03 Mar 2022 17:00
 Operator : SY/VA
 Sample : N1733-13
 Misc : 6.66g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS6

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:34:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		171071	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		167157	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		82039	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		36802	16.494	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	65.960%		
7) Chloroethane-d5	2.879	69		31349	17.857	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	71.440%		
11) 1,1-Dichloroethene-d2	4.013	63		46424	13.586	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	54.360%		
21) 2-Butanone-d5	7.074	46		22038	58.743	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	117.480%		
24) Chloroform-d	7.647	84		87685	22.973	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	91.880%		
26) 1,2-Dichloroethane-d4	8.305	65		46510	23.442	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	93.760%		
32) Benzene-d6	8.275	84		164142	21.099	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	84.400%		
36) 1,2-Dichloropropane-d6	9.275	67		49301	22.820	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	91.280%		
41) Toluene-d8	10.323	98		153684	19.871	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	79.480%		
43) trans-1,3-Dichloroprop...	10.579	79		18546	19.361	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	77.440%		
47) 2-Hexanone-d5	10.921	63		18876	53.122	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	106.240%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		44819	23.638	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	94.560%		
66) 1,2-Dichlorobenzene-d4	13.853	152		63459	24.083	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	96.320%		
Target Compounds							
13) Acetone	4.135	43		1765	5.760	ug/L	71
20) cis-1,2-Dichloroethene	7.165	96		1441m	0.685	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022168.D
Acq On : 03 Mar 2022 17:00
Operator : SY/VA
Sample : N1733-13
Misc : 6.66g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:34:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

