




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022169.D
Acq On : 03 Mar 2022 17:24
Operator : SY/VA
Sample : N1733-14
Misc : 6.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS7

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:35:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

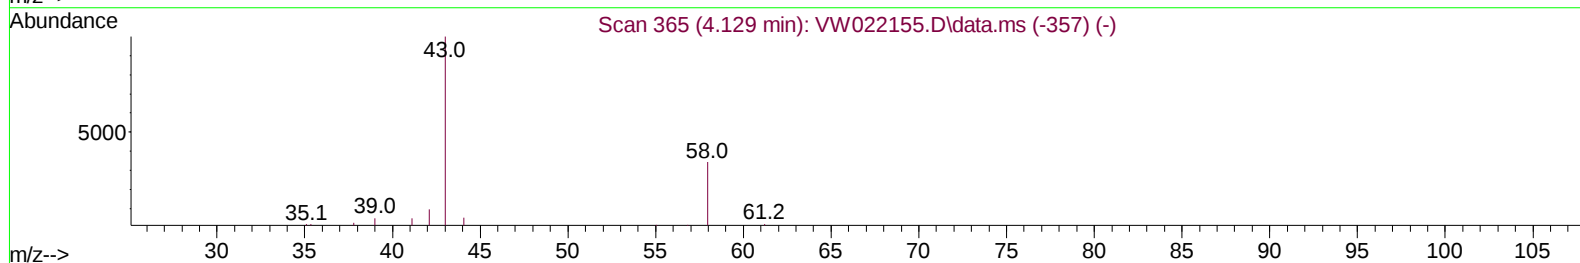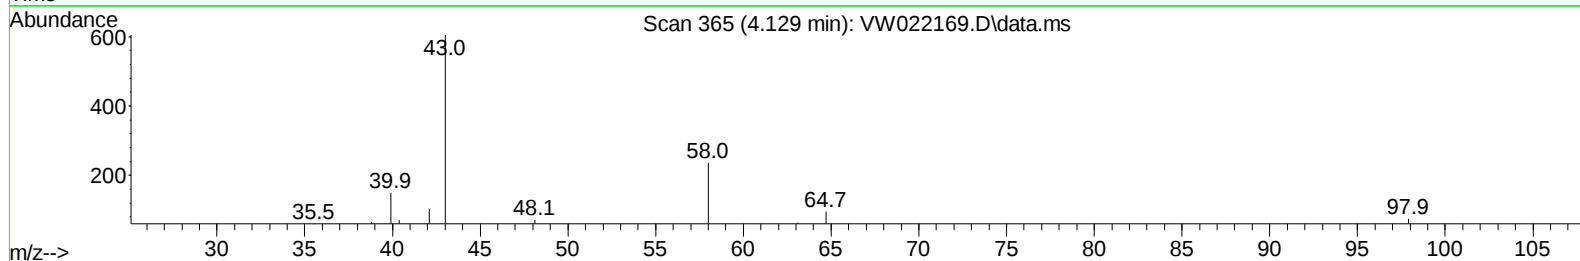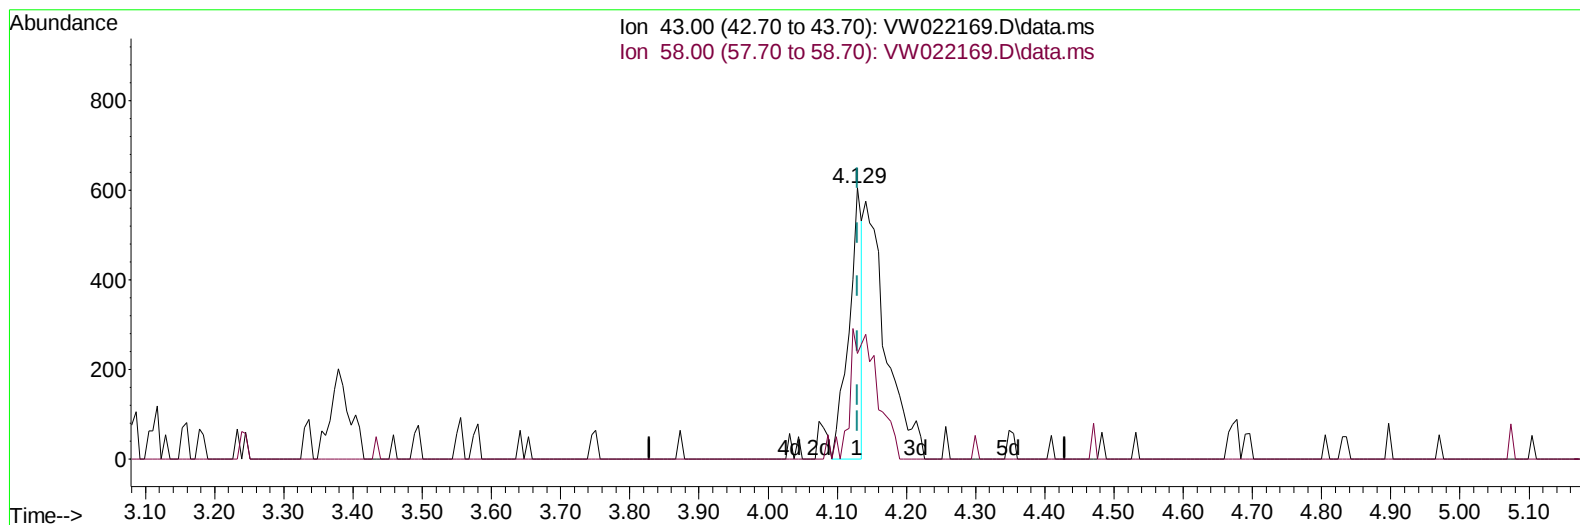

TIC: VW022169.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 2.63 ug/L

response 814

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	29.61
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022169.D
Acq On : 03 Mar 2022 17:24
Operator : SY/VA
Sample : N1733-14
Misc : 6.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS7

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:35:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

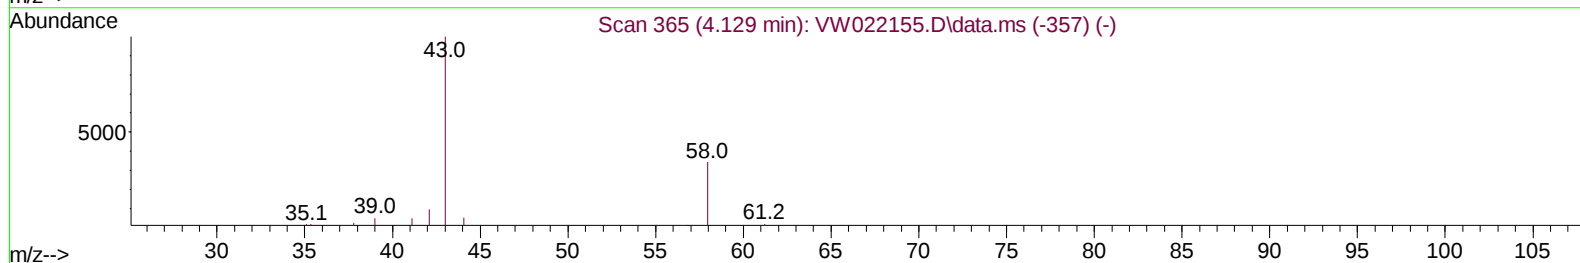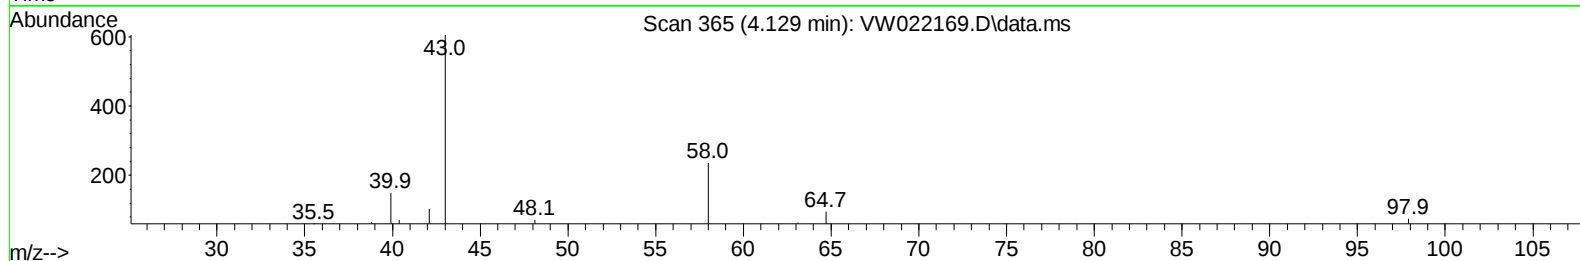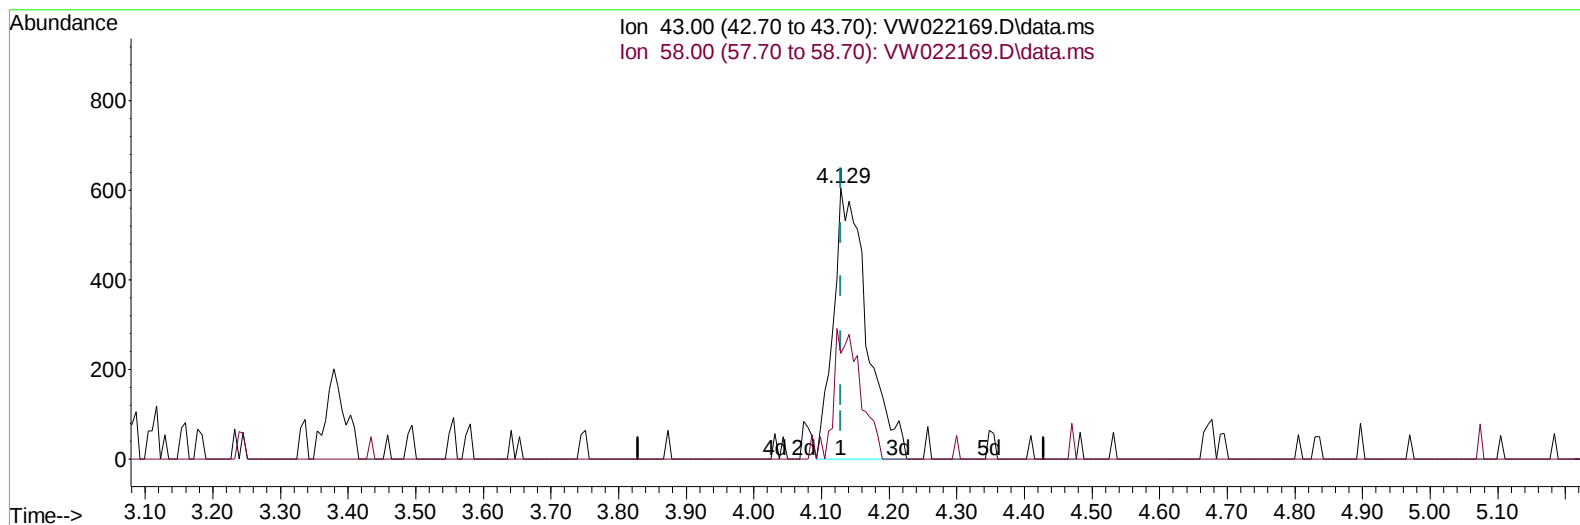

TIC: VW022169.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 6.69 ug/L m

response 2073

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	11.63
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022169.D
 Acq On : 03 Mar 2022 17:24
 Operator : SY/VA
 Sample : N1733-14
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS7

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:35:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	173055	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	165351	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	84581	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	38037	16.852	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.400%	
7) Chloroethane-d5	2.879	69	34417	19.379	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.520%	
11) 1,1-Dichloroethene-d2	4.013	63	48422	14.009	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.040%	
21) 2-Butanone-d5	7.079	46	22005	57.983	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	115.960%	
24) Chloroform-d	7.646	84	92757	24.023	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.080%	
26) 1,2-Dichloroethane-d4	8.305	65	48375	24.103	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	96.400%	
32) Benzene-d6	8.274	84	169235	21.992	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	87.960%	
36) 1,2-Dichloropropane-d6	9.274	67	50322	23.547	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	94.200%	
41) Toluene-d8	10.323	98	160815	21.020	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	84.080%	
43) trans-1,3-Dichloroprop...	10.579	79	19733	20.825	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	83.280%	
47) 2-Hexanone-d5	10.920	63	18990	54.027	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.060%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	46701	24.900	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	99.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152	67476	24.838	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.360%	
Target Compounds						
13) Acetone	4.129	43	2073m	6.688	ug/L	
20) cis-1,2-Dichloroethene	7.159	96	2106	0.990	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022169.D
Acq On : 03 Mar 2022 17:24
Operator : SY/VA
Sample : N1733-14
Misc : 6.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRS7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:35:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

