




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022170.D
 Acq On : 03 Mar 2022 17:48
 Operator : SY/VA
 Sample : N1733-19
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRT7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:35:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

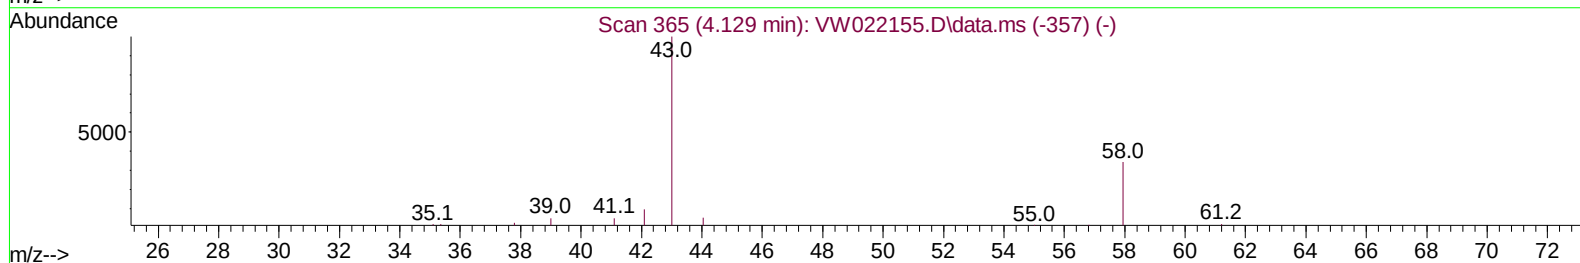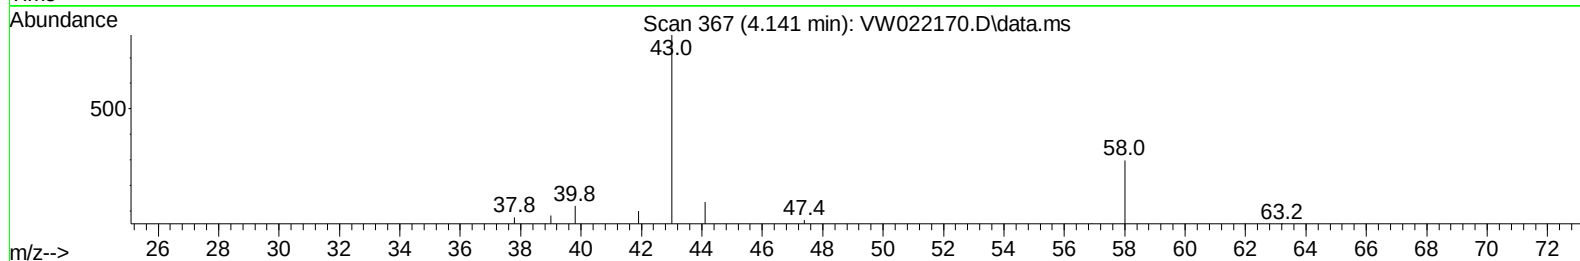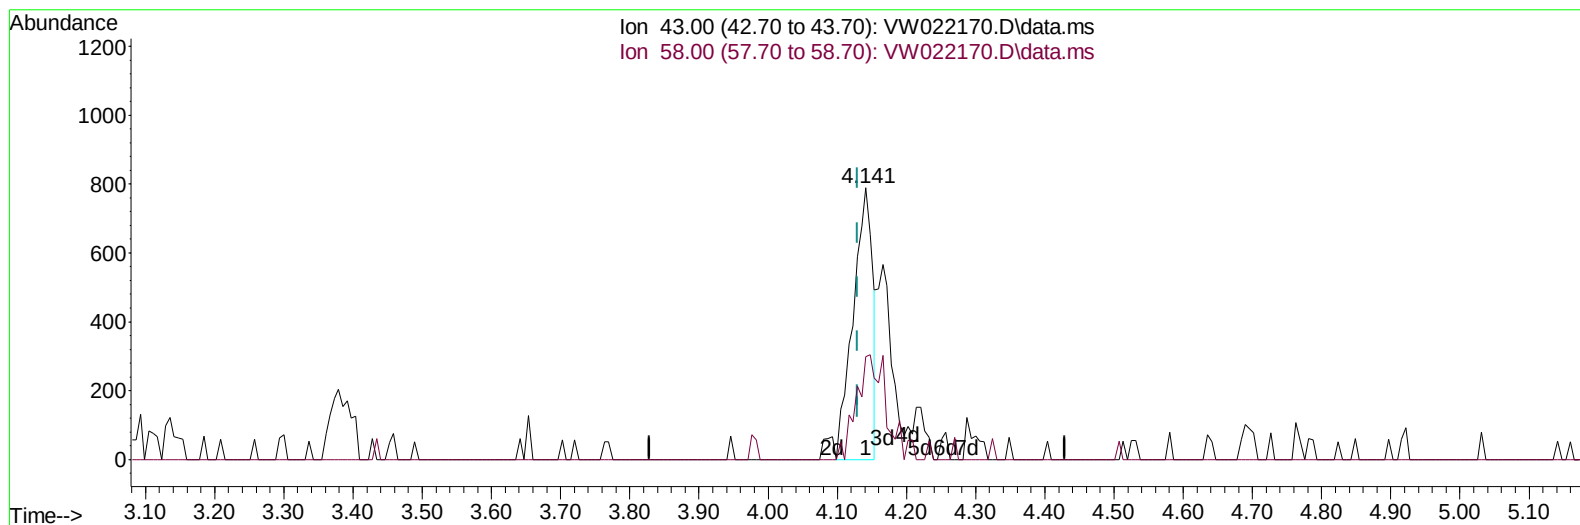

TIC: VW022170.D\data.ms

(13) Acetone (T)

4.141min (+ 0.012) 4.84 ug/L

response 1558

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	39.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022170.D
 Acq On : 03 Mar 2022 17:48
 Operator : SY/VA
 Sample : N1733-19
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRT7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:35:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

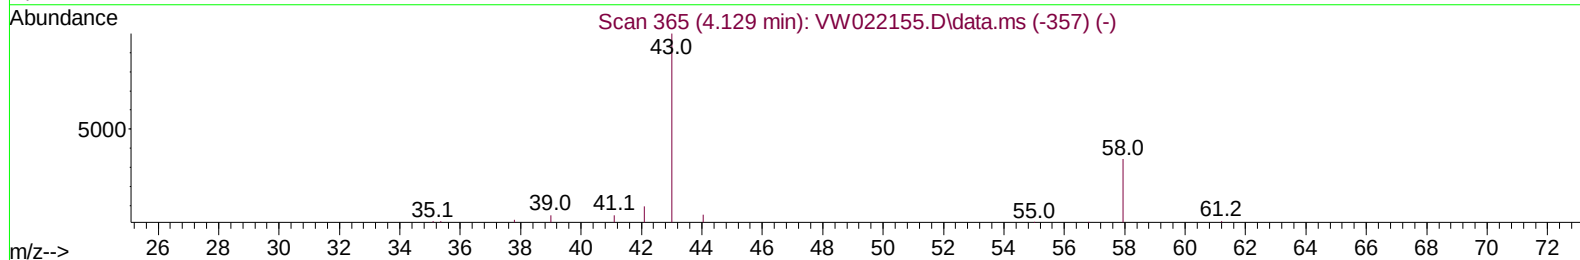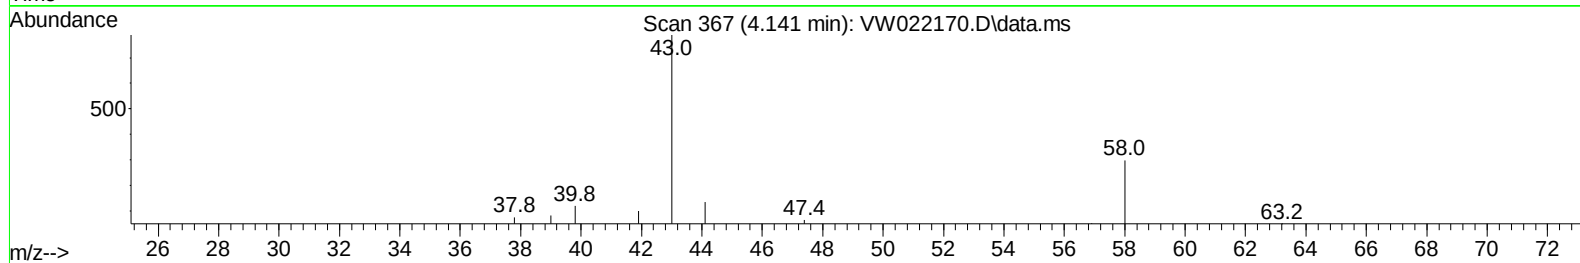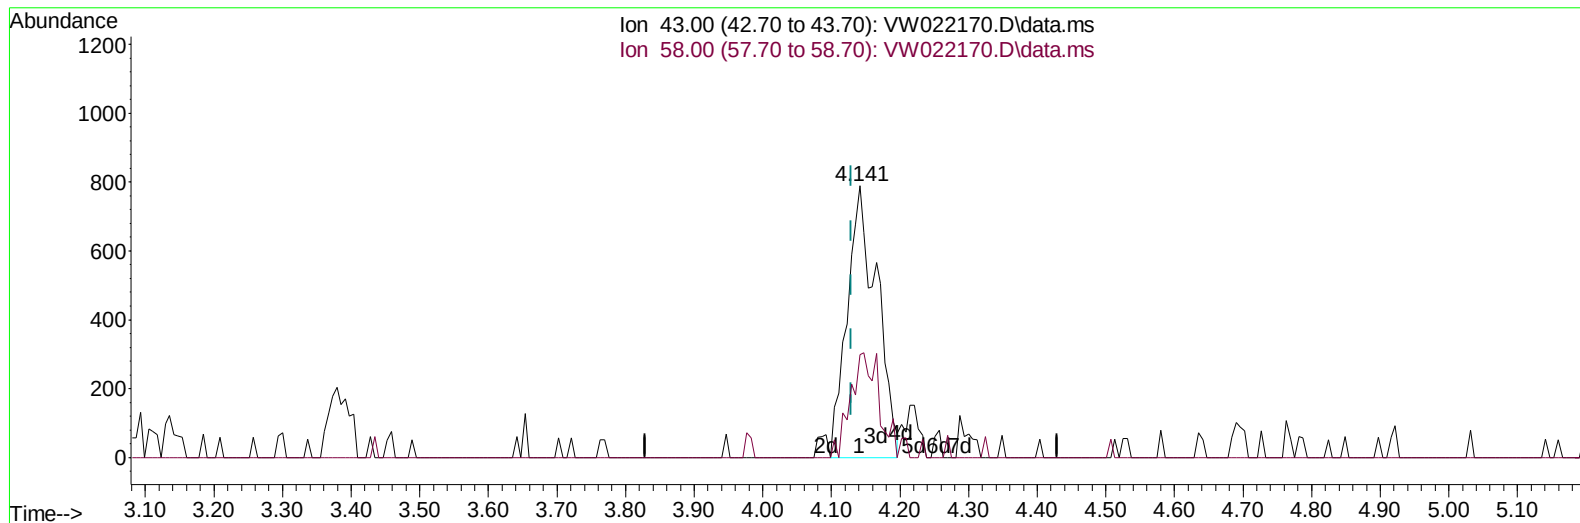

TIC: VW022170.D\data.ms

(13) Acetone (T)

4.141min (+ 0.012) 7.37 ug/L m

response 2374

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	26.16
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022170.D
 Acq On : 03 Mar 2022 17:48
 Operator : SY/VA
 Sample : N1733-19
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRT7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:35:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		179867	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		168988	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		88157	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		39195	16.707	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	66.840%		
7) Chloroethane-d5	2.879	69		33938	18.386	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	73.560%		
11) 1,1-Dichloroethene-d2	4.013	63		49542	13.790	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	55.160%		
21) 2-Butanone-d5	7.080	46		22311	56.562	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	113.120%		
24) Chloroform-d	7.647	84		91815	22.879	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	91.520%		
26) 1,2-Dichloroethane-d4	8.305	65		49538	23.747	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	95.000%		
32) Benzene-d6	8.275	84		171800	21.844	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	87.360%		
36) 1,2-Dichloropropane-d6	9.274	67		51351	23.511	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	94.040%		
41) Toluene-d8	10.323	98		161823	20.696	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	82.800%		
43) trans-1,3-Dichloroprop...	10.579	79		19527	20.164	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	80.640%		
47) 2-Hexanone-d5	10.921	63		19924	55.464	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	110.920%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		48508	25.307	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	101.240%		
66) 1,2-Dichlorobenzene-d4	13.853	152		65061	22.977	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	91.920%		
Target Compounds							
13) Acetone	4.141	43		2374m	7.369	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022170.D
Acq On : 03 Mar 2022 17:48
Operator : SY/VA
Sample : N1733-19
Misc : 6.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRT7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:35:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

