

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022166.D
 Acq On : 03 Mar 2022 16:12
 Operator : SY/VA
 Sample : N1733-08
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:34:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	134027	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	126245	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	60898	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	31114	17.798	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.200%		
7) Chloroethane-d5	2.879	69	26659	19.382	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.520%		
11) 1,1-Dichloroethene-d2	4.013	63	37665	14.070	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.280%		
21) 2-Butanone-d5	7.080	46	17764	60.438	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	120.880%		
24) Chloroform-d	7.647	84	69995	23.407	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.640%		
26) 1,2-Dichloroethane-d4	8.305	65	37611	24.196	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	96.800%		
32) Benzene-d6	8.275	84	128381	21.850	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.400%		
36) 1,2-Dichloropropane-d6	9.275	67	38630	23.675	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.720%		
41) Toluene-d8	10.323	98	121370	20.778	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	83.120%		
43) trans-1,3-Dichloroprop...	10.573	79	14664	20.269	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.080%		
47) 2-Hexanone-d5	10.921	63	15007	55.920	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	111.840%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	36008	25.146	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.600%		
66) 1,2-Dichlorobenzene-d4	13.853	152	51261	26.207	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	104.840%		
Target Compounds					Qvalue	
13) Acetone	4.154	43	1741m	7.252	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022166.D
Acq On : 03 Mar 2022 16:12
Operator : SY/VA
Sample : N1733-08
Misc : 4.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBRS3

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022


Quant Time: Mar 04 00:34:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

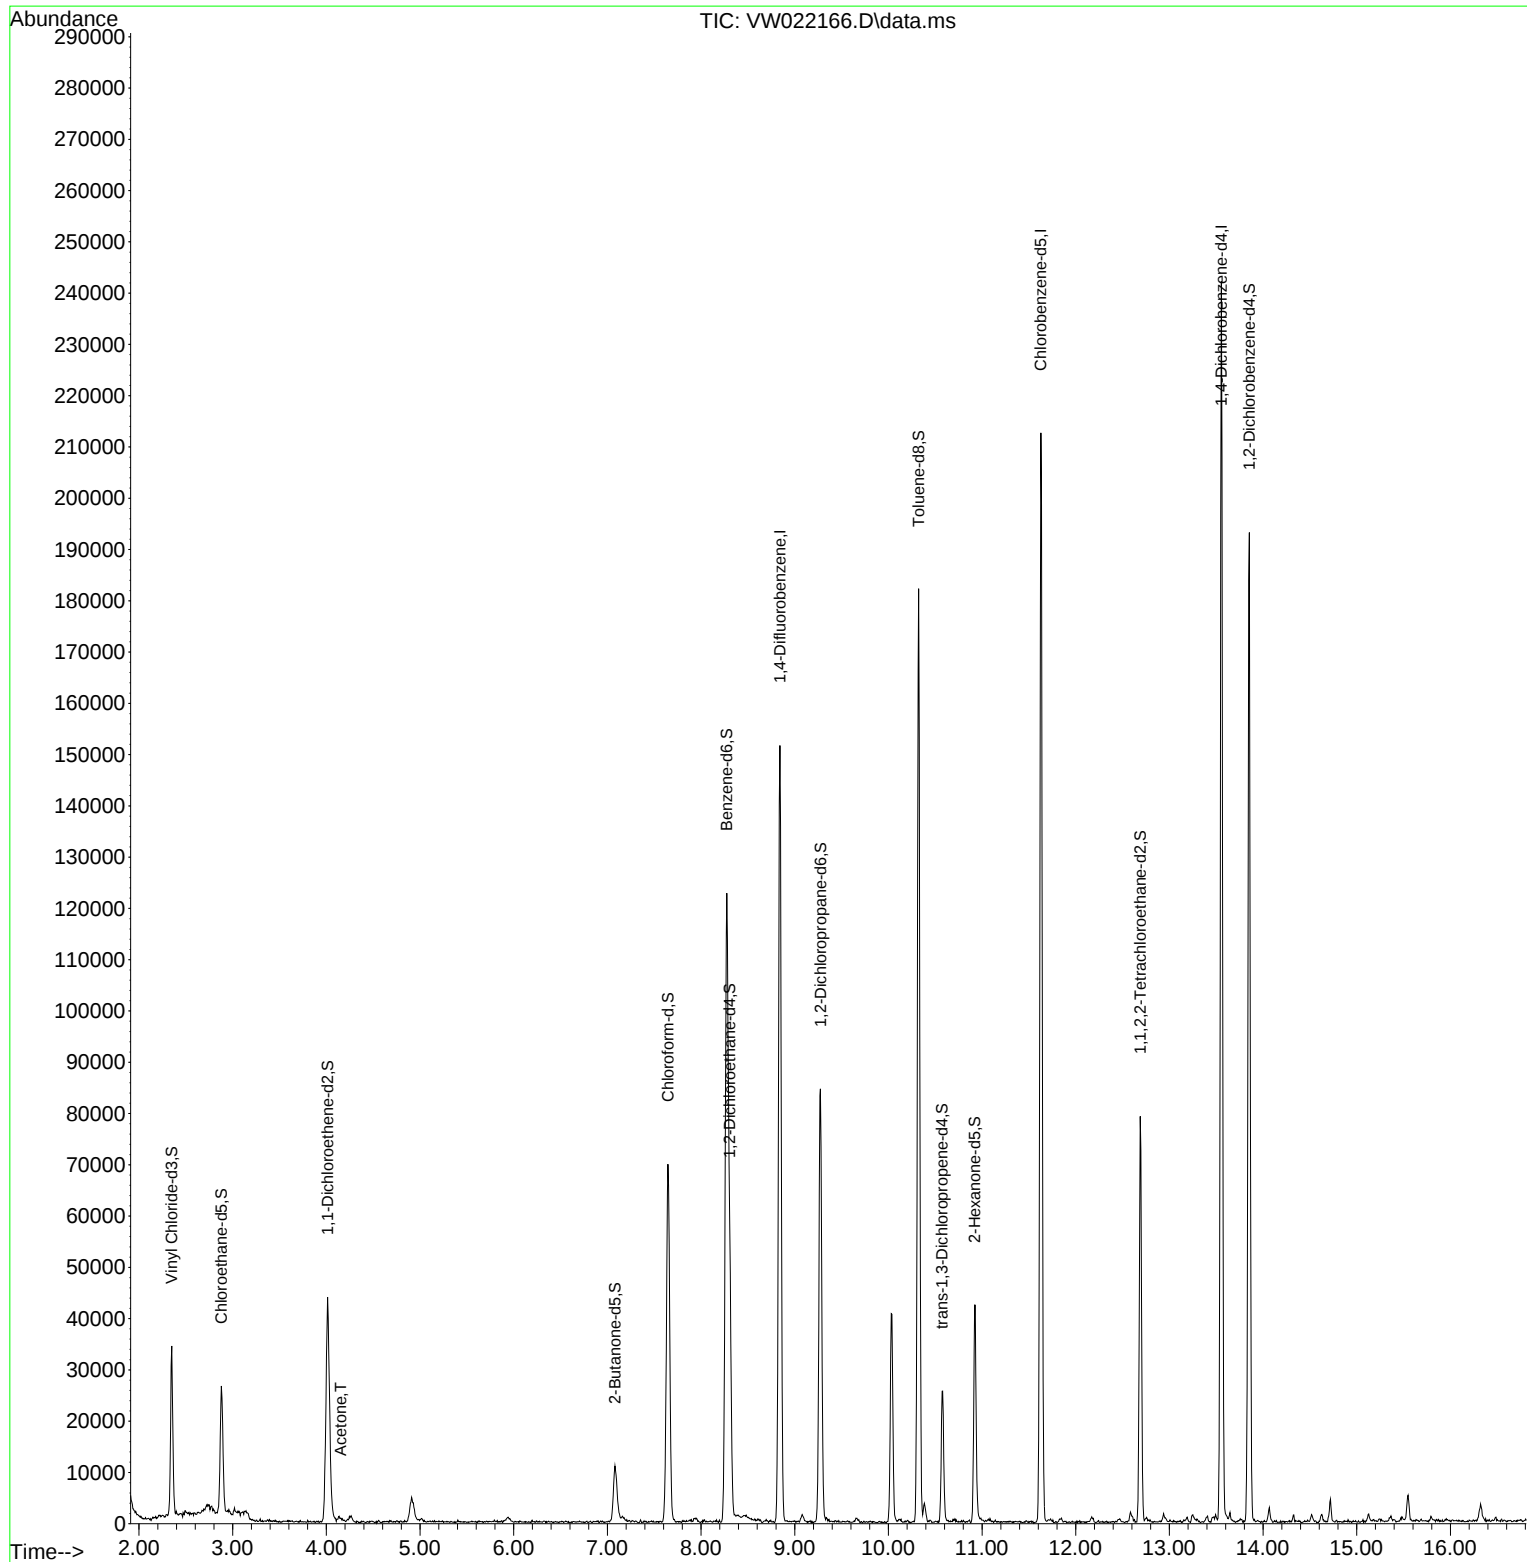

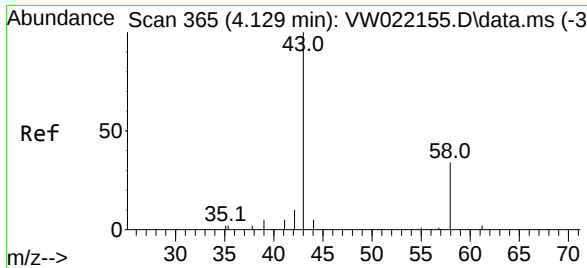

#13
 Acetone
 Concen: 7.252 ug/L m
 RT: 4.154 min Scan# 30
 Delta R.T. 0.025 min
 Lab File: VW022166.D
 Acq: 03 Mar 2022 16:12

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRS3

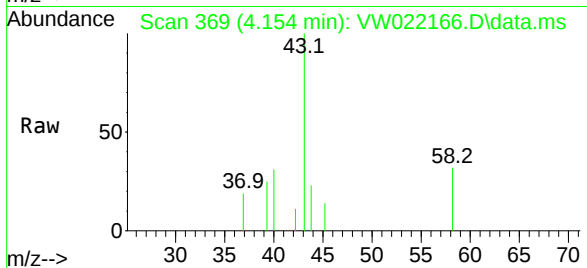

Tgt Ion: 43 Resp: 174
 Ion Ratio Lower Upper
 43 100
 58 23.4 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

