

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022170.D
 Acq On : 03 Mar 2022 17:48
 Operator : SY/VA
 Sample : N1733-19
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRT7

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 04 00:35:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	179867	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	168988	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	88157	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	39195	16.707	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.840%		
7) Chloroethane-d5	2.879	69	33938	18.386	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.560%		
11) 1,1-Dichloroethene-d2	4.013	63	49542	13.790	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	55.160%		
21) 2-Butanone-d5	7.080	46	22311	56.562	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	113.120%		
24) Chloroform-d	7.647	84	91815	22.879	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.520%		
26) 1,2-Dichloroethane-d4	8.305	65	49538	23.747	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.000%		
32) Benzene-d6	8.275	84	171800	21.844	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.360%		
36) 1,2-Dichloropropane-d6	9.274	67	51351	23.511	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.040%		
41) Toluene-d8	10.323	98	161823	20.696	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.800%		
43) trans-1,3-Dichloroprop...	10.579	79	19527	20.164	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.640%		
47) 2-Hexanone-d5	10.921	63	19924	55.464	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.920%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	48508	25.307	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.240%		
66) 1,2-Dichlorobenzene-d4	13.853	152	65061	22.977	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.920%		
Target Compounds					Qvalue	
13) Acetone	4.141	43	2374m	7.369	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022170.D
Acq On : 03 Mar 2022 17:48
Operator : SY/VA
Sample : N1733-19
Misc : 6.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBRT7

Quant Time: Mar 04 00:35:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

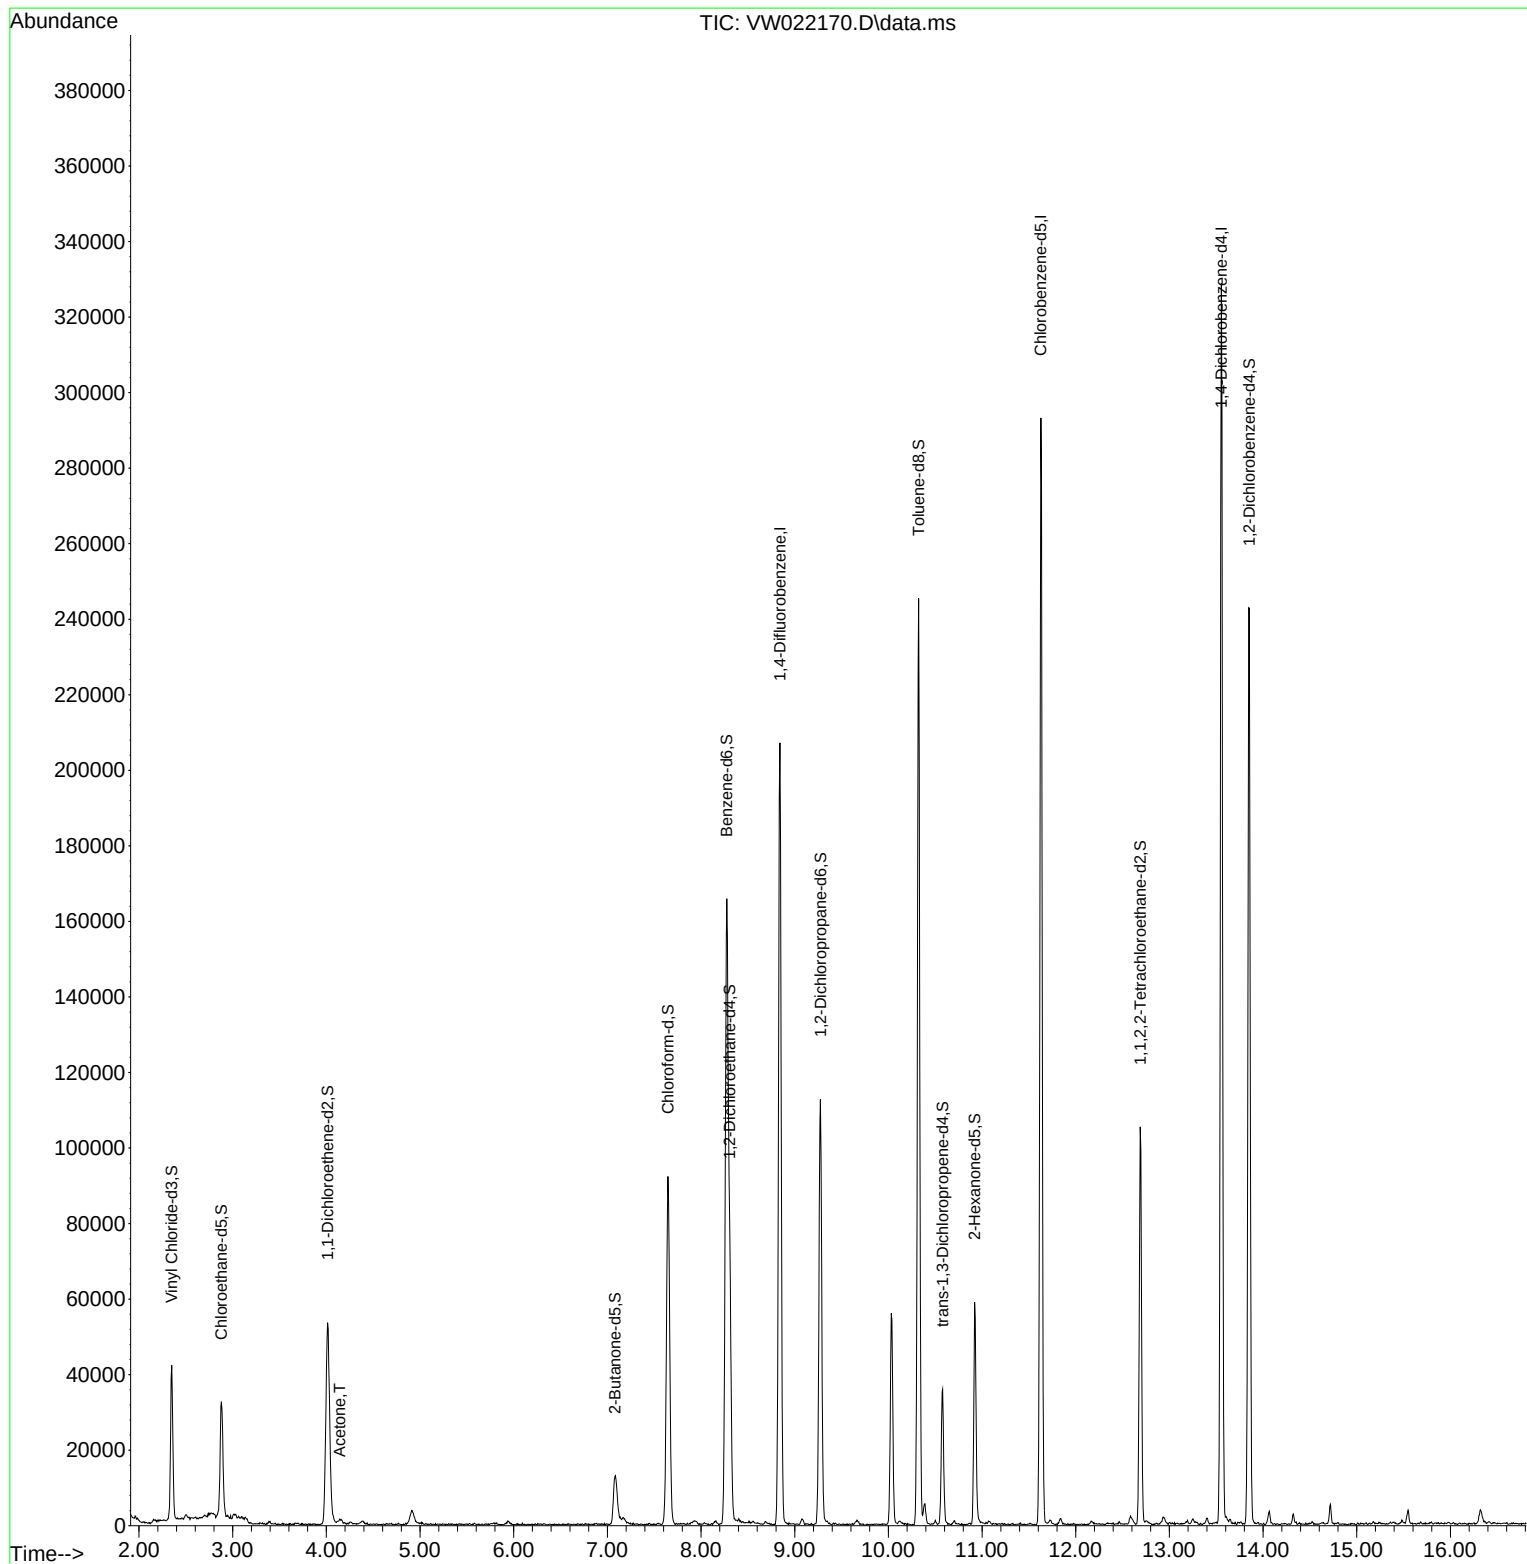

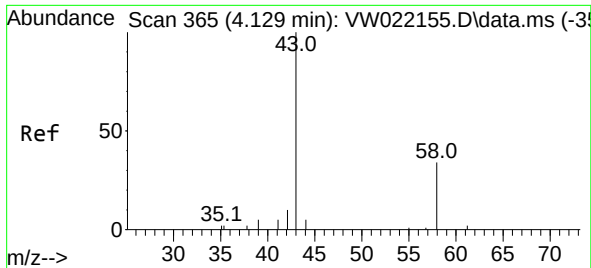

#13
 Acetone
 Concen: 7.369 ug/L m
 RT: 4.141 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW022170.D
 Acq: 03 Mar 2022 17:48

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRT7

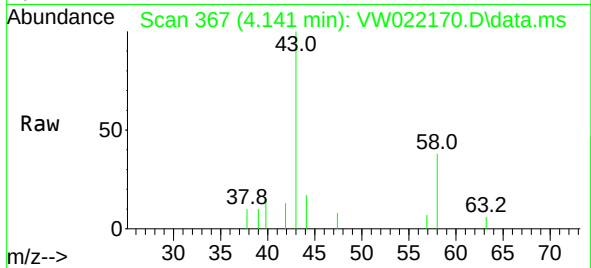

Tgt Ion: 43 Resp: 2374
 Ion Ratio Lower Upper
 43 100
 58 26.2 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

