
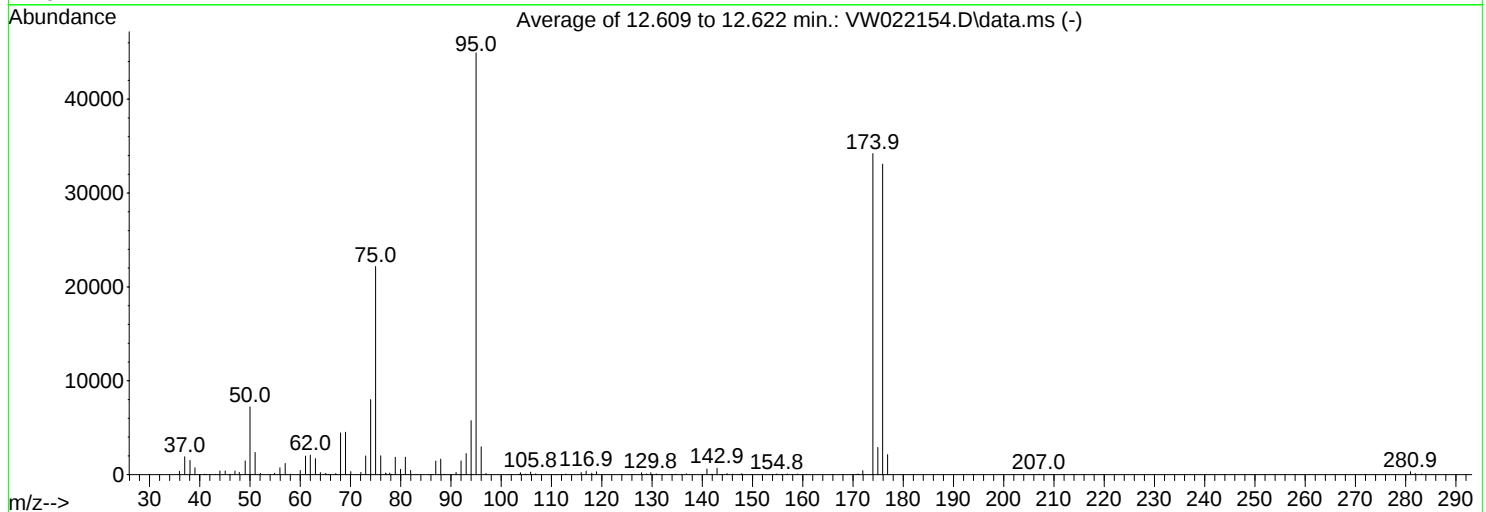


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022154.D
 Acq On : 03 Mar 2022 07:52
 Operator : SY/VA
 Sample : BFB515
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB515

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Title : SFAM01.0
 Last Update : Sat Mar 05 03:21:21 2022

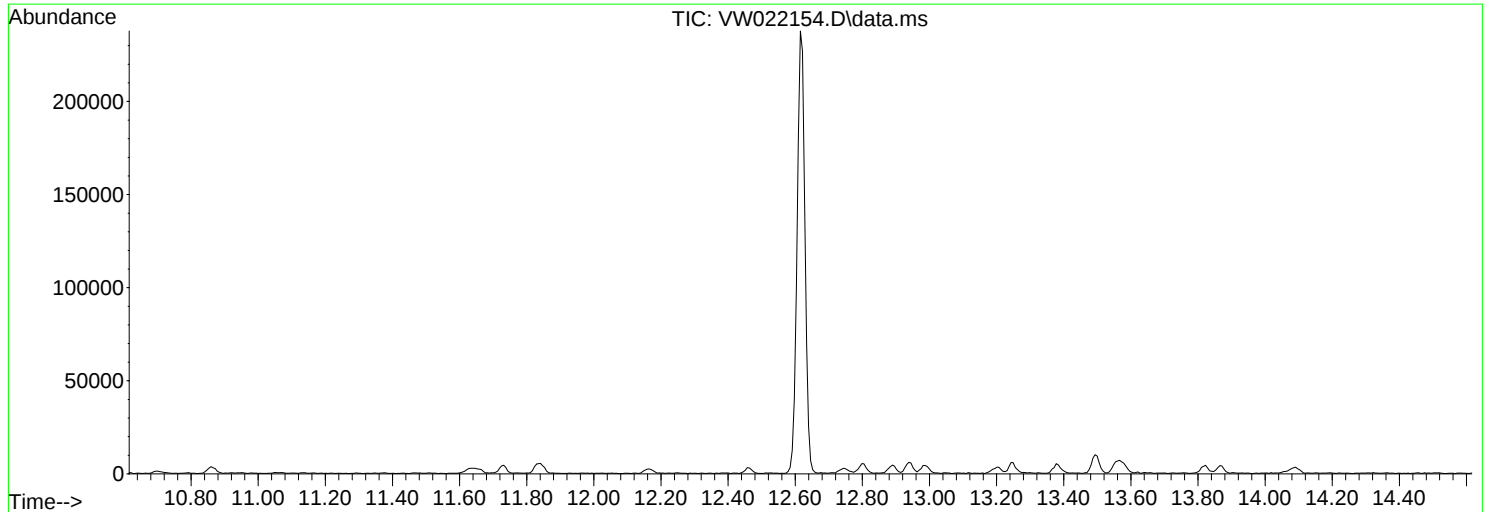

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	7221	PASS
75	95	30	80	49.3	22168	PASS
95	95	100	100	100.0	44931	PASS
96	95	5	9	6.6	2965	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.1	34205	PASS
175	174	5	9	8.5	2904	PASS
176	174	95	105	96.7	33083	PASS
177	176	5	10	6.4	2132	PASS

m/z	Abundance
39.90	172.0
57.10	61.0
70.30	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB515

m/z	Abundance
36.00	269.0
37.00	1901.0
38.00	1441.0
39.10	735.0
40.00	157.0
41.30	78.0
43.10	59.0
44.00	413.0
45.00	438.0
47.10	480.0
48.00	257.0
49.10	1288.0
50.00	6251.0
51.00	2272.0
52.10	193.0
55.00	178.0
56.00	615.0
57.00	1134.0
58.00	54.0
60.00	397.0
61.10	1715.0
62.00	1697.0
63.00	1606.0
64.00	217.0
65.00	190.0
67.00	115.0
68.00	4009.0
69.00	3954.0
70.00	368.0
72.00	245.0
73.00	1784.0
74.00	6648.0
75.00	18632.0
76.00	1766.0
77.10	266.0
77.90	157.0
78.90	1762.0
79.90	436.0
80.90	1568.0
81.90	370.0
86.90	1323.0
87.90	1411.0
88.70	118.0
91.00	152.0
92.00	1091.0
93.00	1849.0
94.00	5219.0
95.00	38920.0
96.00	2363.0
97.00	114.0
103.70	232.0
104.80	118.0
105.80	261.0
106.90	97.0
112.80	62.0
115.80	142.0
116.90	365.0
118.00	178.0
118.90	263.0
127.80	170.0
129.00	68.0
129.70	213.0
130.80	71.0
134.80	101.0
136.80	81.0
140.90	460.0
141.80	84.0
143.00	621.0
144.90	158.0
147.80	59.0
156.70	61.0
159.00	62.0
160.70	86.0
171.10	78.0
171.90	378.0
173.90	27096.0
175.00	2271.0
175.90	23872.0
176.90	1824.0
207.00	132.0
281.00	431.0
281.90	179.0
283.20	92.0

Instrument :
MSVOA_W
ClientSampleId :
BFB515

m/z	Abundance
36.00	354.0
37.00	2084.0
38.00	1662.0
39.00	815.0
39.90	170.0
40.90	53.0
43.20	68.0
44.00	449.0
45.10	443.0
46.00	77.0
46.90	409.0
47.80	219.0
49.00	1616.0
50.00	8203.0
51.00	2456.0
52.10	162.0
54.80	213.0
56.00	850.0
57.00	1324.0
58.00	56.0
60.00	469.0
61.00	2009.0
62.00	2278.0
63.00	1984.0
64.10	221.0
65.20	186.0
65.70	51.0
67.00	210.0
68.00	4906.0
69.00	4835.0
70.10	464.0
72.10	231.0
73.00	2438.0
74.00	9335.0
75.00	25672.0
76.00	2279.0
76.90	240.0
77.70	198.0
78.90	1986.0
80.00	689.0
80.90	2202.0
82.00	458.0
83.00	59.0
87.00	1575.0
88.00	1773.0
91.00	348.0
92.00	1858.0
93.10	2528.0
94.00	6464.0
95.00	50576.0
96.00	3360.0
96.90	159.0
103.90	338.0
104.80	98.0
105.90	288.0
106.90	105.0
110.90	53.0
112.90	52.0
115.90	159.0
116.90	459.0
118.00	154.0
118.90	380.0
127.90	271.0
128.90	117.0
129.70	201.0
130.90	83.0
134.60	57.0
136.90	91.0
141.00	700.0
142.00	118.0
142.90	691.0
144.90	65.0
146.00	77.0
147.80	181.0
149.80	52.0
154.80	86.0
155.70	56.0
157.00	146.0
158.60	68.0
159.10	51.0
160.80	72.0
171.00	151.0
171.90	531.0
173.90	36280.0
175.00	3198.0
175.90	35712.0
176.90	2293.0
178.00	78.0
207.00	51.0
280.90	326.0
282.00	97.0
283.10	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB515

m/z	Abundance
35.90	429.0
37.00	1744.0
38.10	1455.0
39.10	646.0
39.90	153.0
41.00	78.0
44.00	299.0
45.10	279.0
46.00	106.0
47.00	292.0
47.80	238.0
49.00	1502.0
50.00	7210.0
51.00	2393.0
51.90	77.0
55.00	89.0
55.90	715.0
57.00	1294.0
58.00	84.0
60.00	458.0
61.00	2189.0
62.00	2281.0
63.00	1547.0
63.90	203.0
65.00	161.0
65.70	59.0
67.20	159.0
68.00	4457.0
69.00	4754.0
70.00	308.0
71.00	76.0
72.00	221.0
73.00	1786.0
74.00	8019.0
75.00	22200.0
76.00	1980.0
77.20	194.0
77.80	140.0
78.10	155.0
78.90	1814.0
80.00	561.0
80.90	1791.0
81.90	532.0
83.10	60.0
85.70	55.0
86.90	1433.0
88.00	1760.0
91.00	236.0
92.00	1464.0
92.90	2348.0
94.00	5600.0
95.00	45296.0
96.00	3173.0
96.90	127.0
103.80	255.0
105.10	88.0
105.80	286.0
106.80	116.0
111.00	62.0
112.10	73.0
112.90	86.0
115.90	343.0
116.90	292.0
118.00	136.0
119.00	302.0
128.00	184.0
128.90	69.0
129.80	225.0
130.80	86.0
136.90	145.0
140.10	54.0
140.90	618.0
142.90	714.0
143.80	66.0
145.00	124.0
146.10	114.0
148.00	154.0
149.90	51.0
152.70	72.0
154.90	181.0
156.90	101.0
158.90	81.0
170.80	147.0
172.00	388.0
174.00	39240.0
174.90	3243.0
175.90	39664.0
176.90	2279.0
280.90	197.0
281.80	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB515