


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW030519\
Data File : VW008968.D
Acq On : 04 Mar 2019 17:57
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W022119S.M
Title : SW846 8260
Last Update : Fri Feb 22 00:38:32 2019

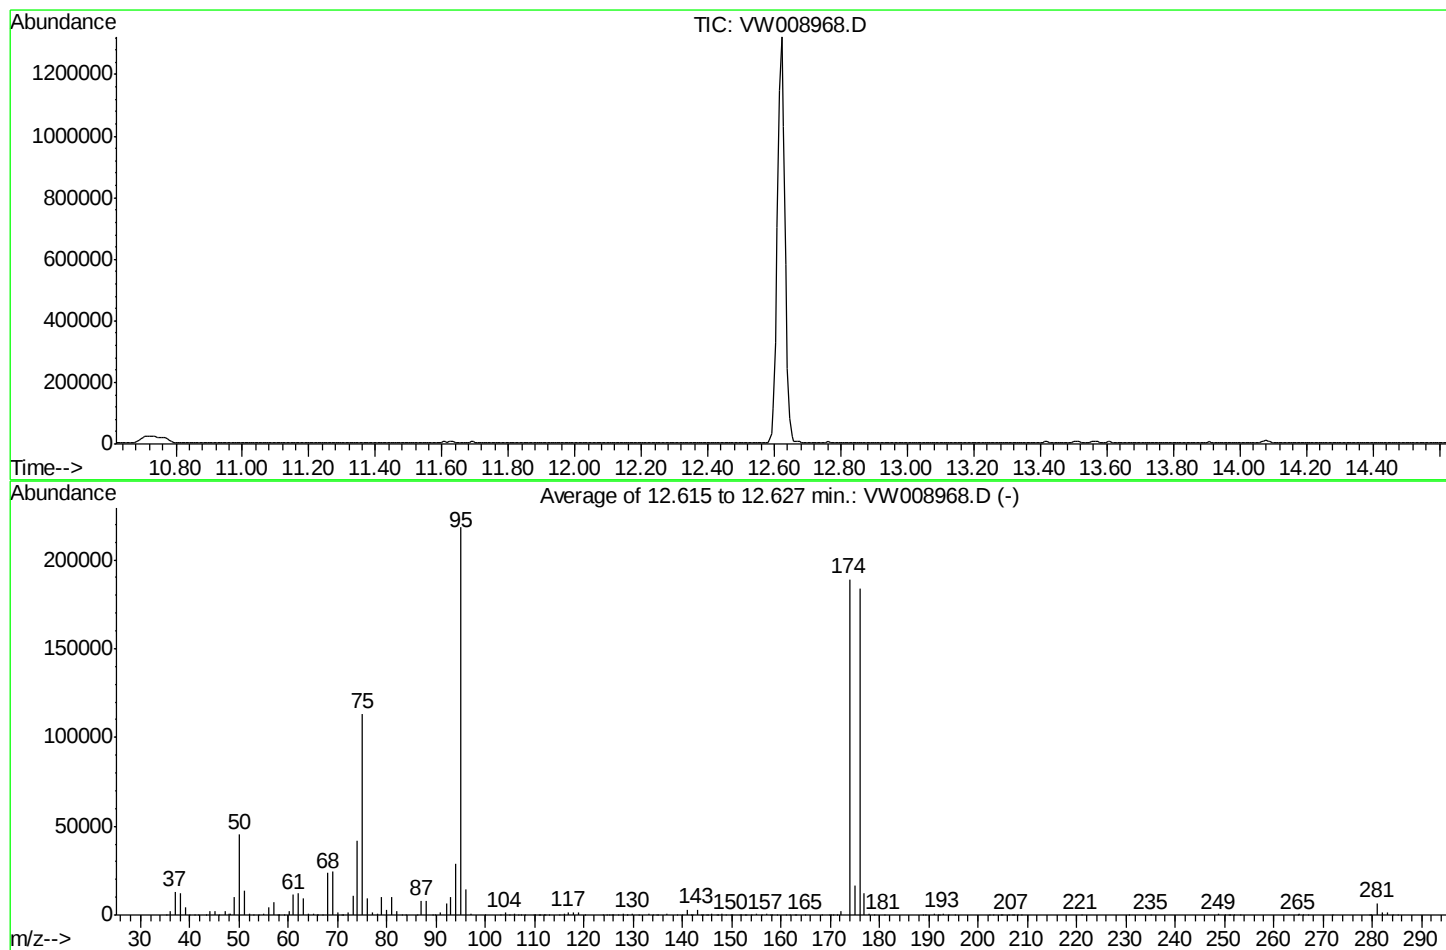

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	45085	PASS
75	95	30	60	52.0	113445	PASS
95	95	100	100	100.0	218282	PASS
96	95	5	9	6.8	14789	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.7	189184	PASS
175	174	5	9	8.6	16310	PASS
176	174	95	101	97.0	183573	PASS
177	176	5	9	6.6	12063	PASS