


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW030519\
 Data File : VW008987.D
 Acq On : 05 Mar 2019 09:52
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W022119S.M
 Title : SW846 8260
 Last Update : Fri Feb 22 00:38:32 2019

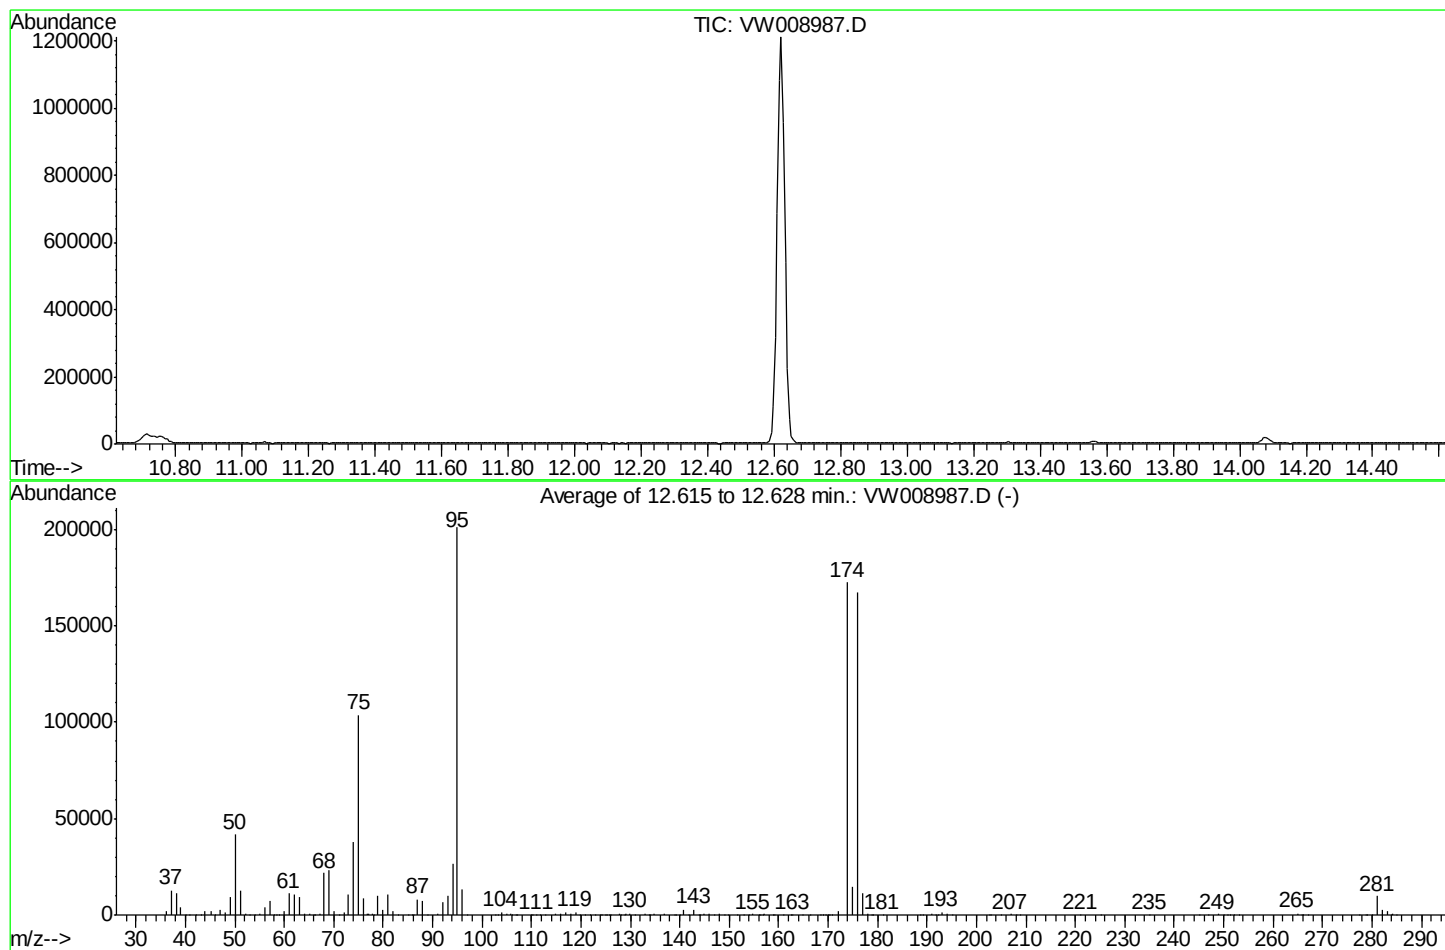

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	41680	PASS
75	95	30	60	51.6	103677	PASS
95	95	100	100	100.0	201066	PASS
96	95	5	9	6.6	13287	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.8	172544	PASS
175	174	5	9	8.4	14521	PASS
176	174	95	101	97.1	167509	PASS
177	176	5	9	6.8	11399	PASS