



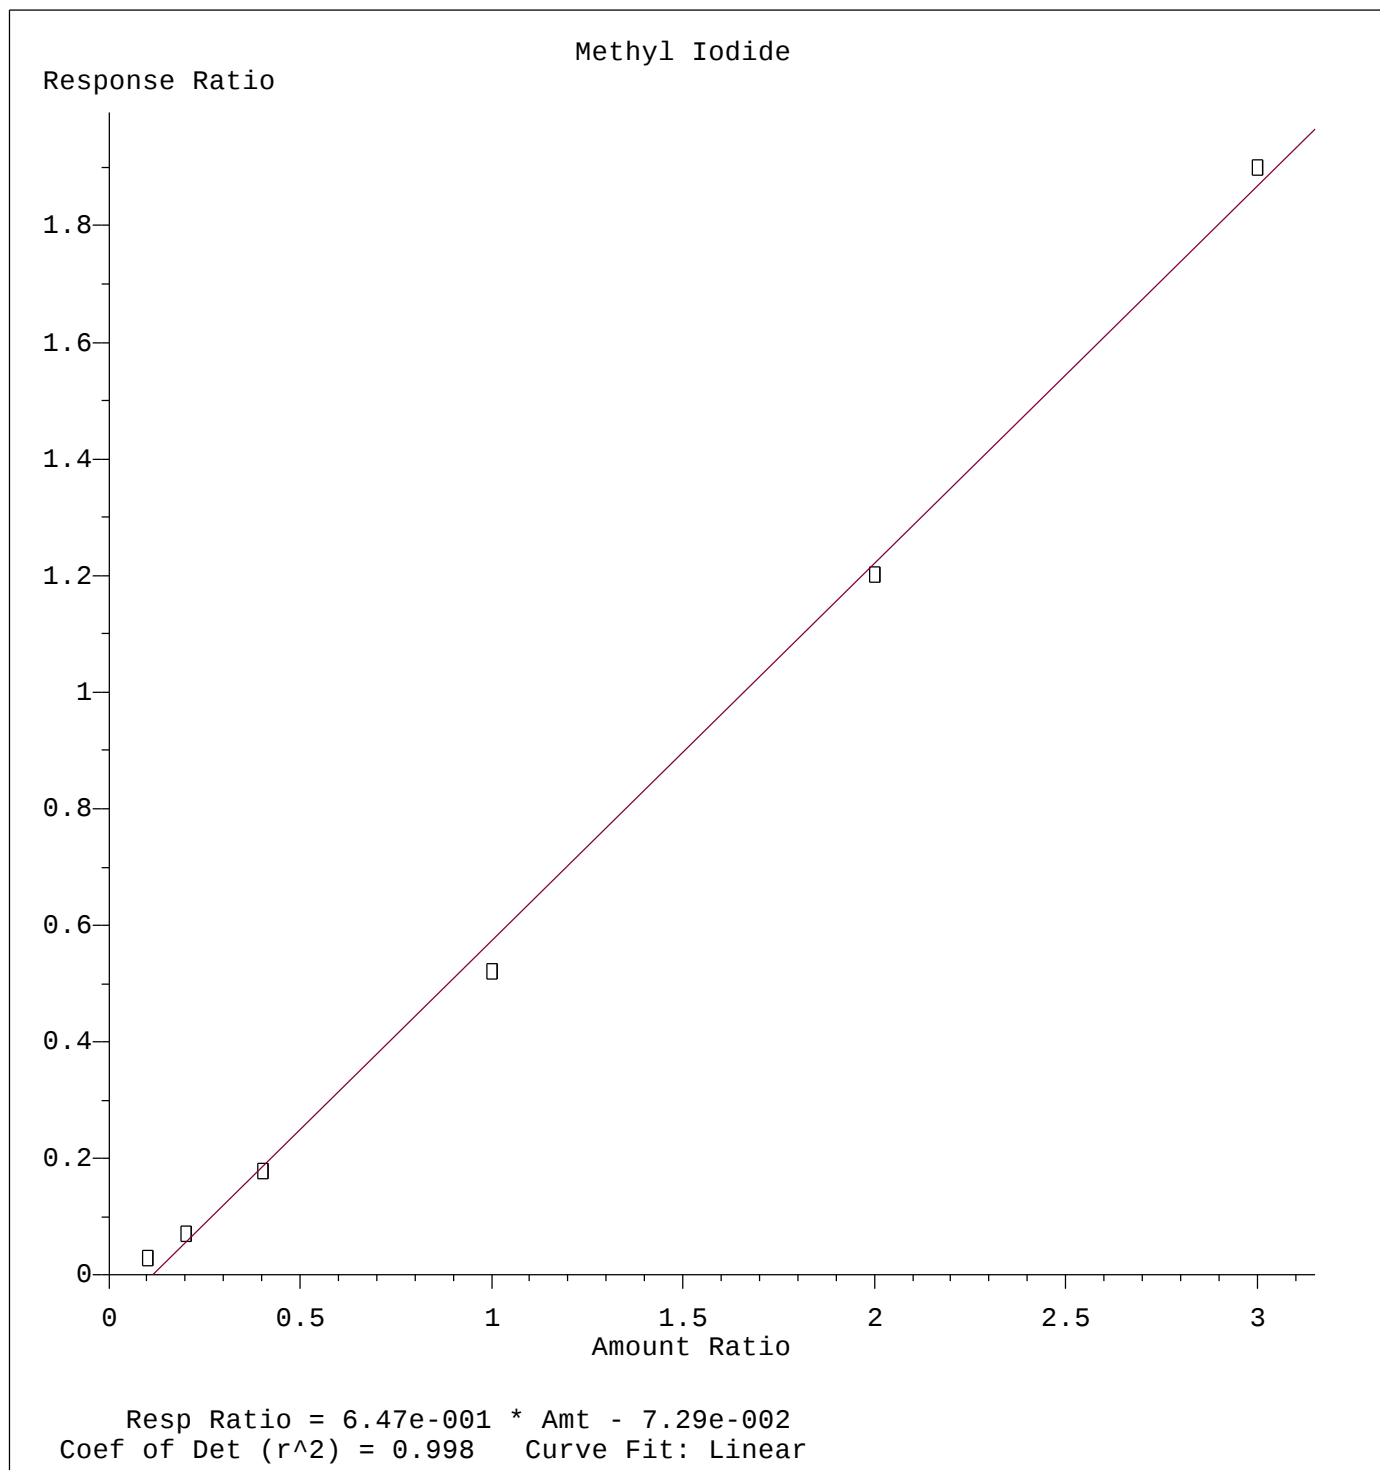

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030619S.M
Calibration Table Last Updated: Thu Mar 07 07:22:06 2019


Methylene Chloride

Response Ratio

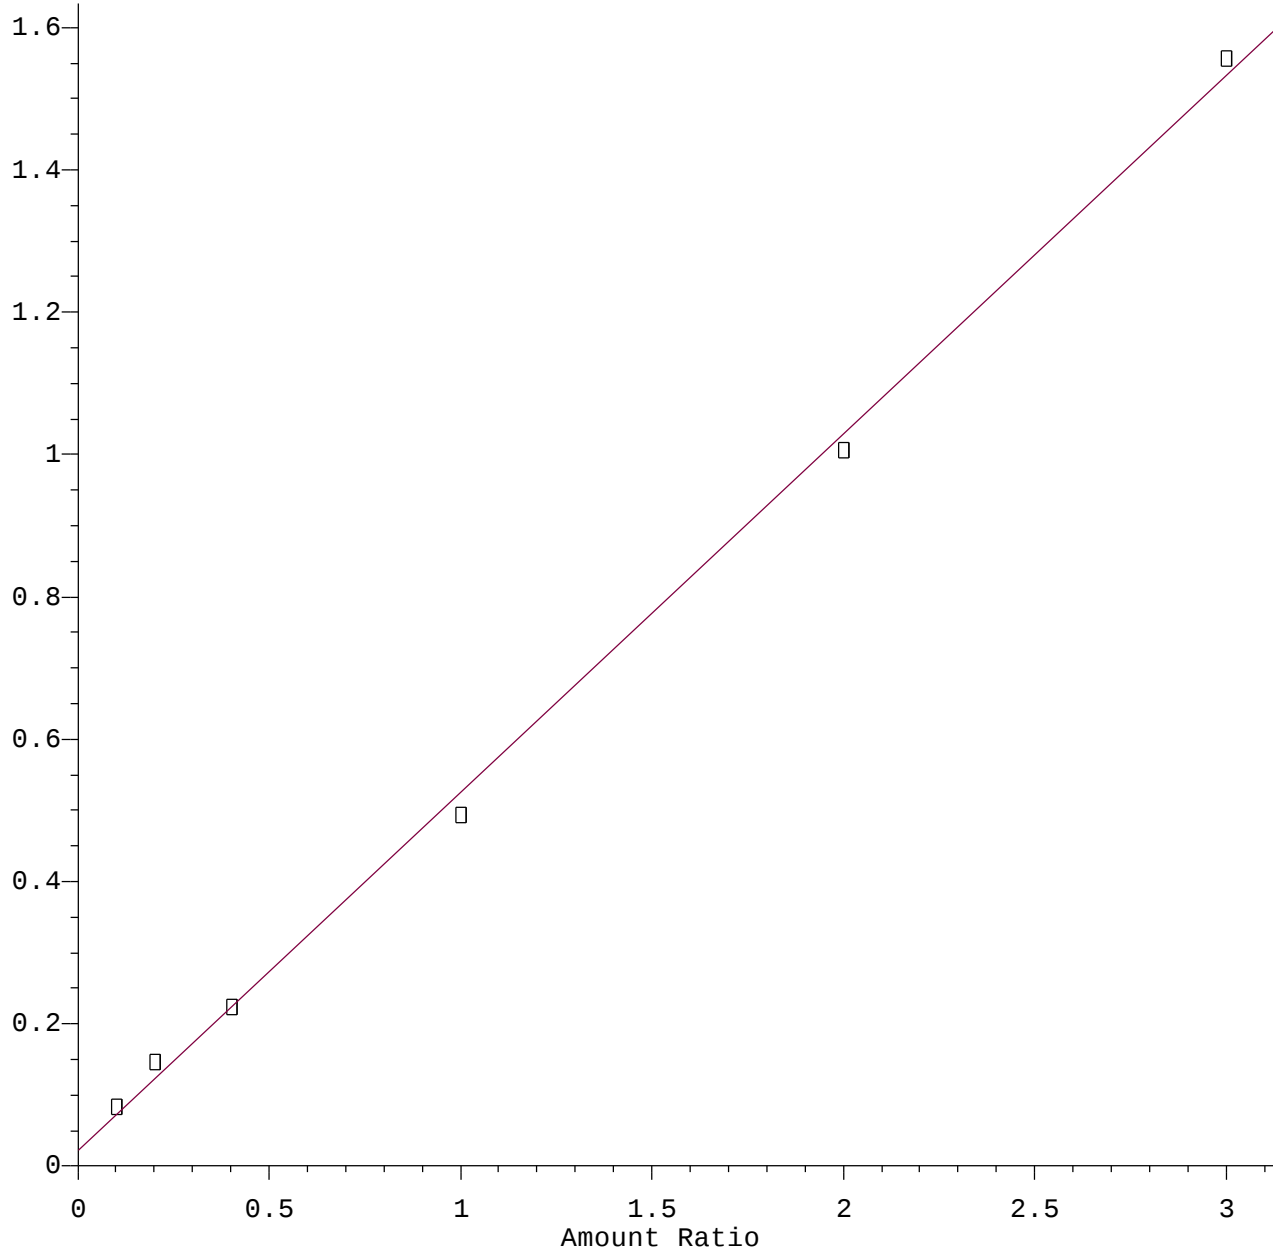


Resp Ratio = $5.03 \times 10^{-1} \times \text{Amt} + 2.21 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030619S.M
Calibration Table Last Updated: Thu Mar 07 07:22:06 2019

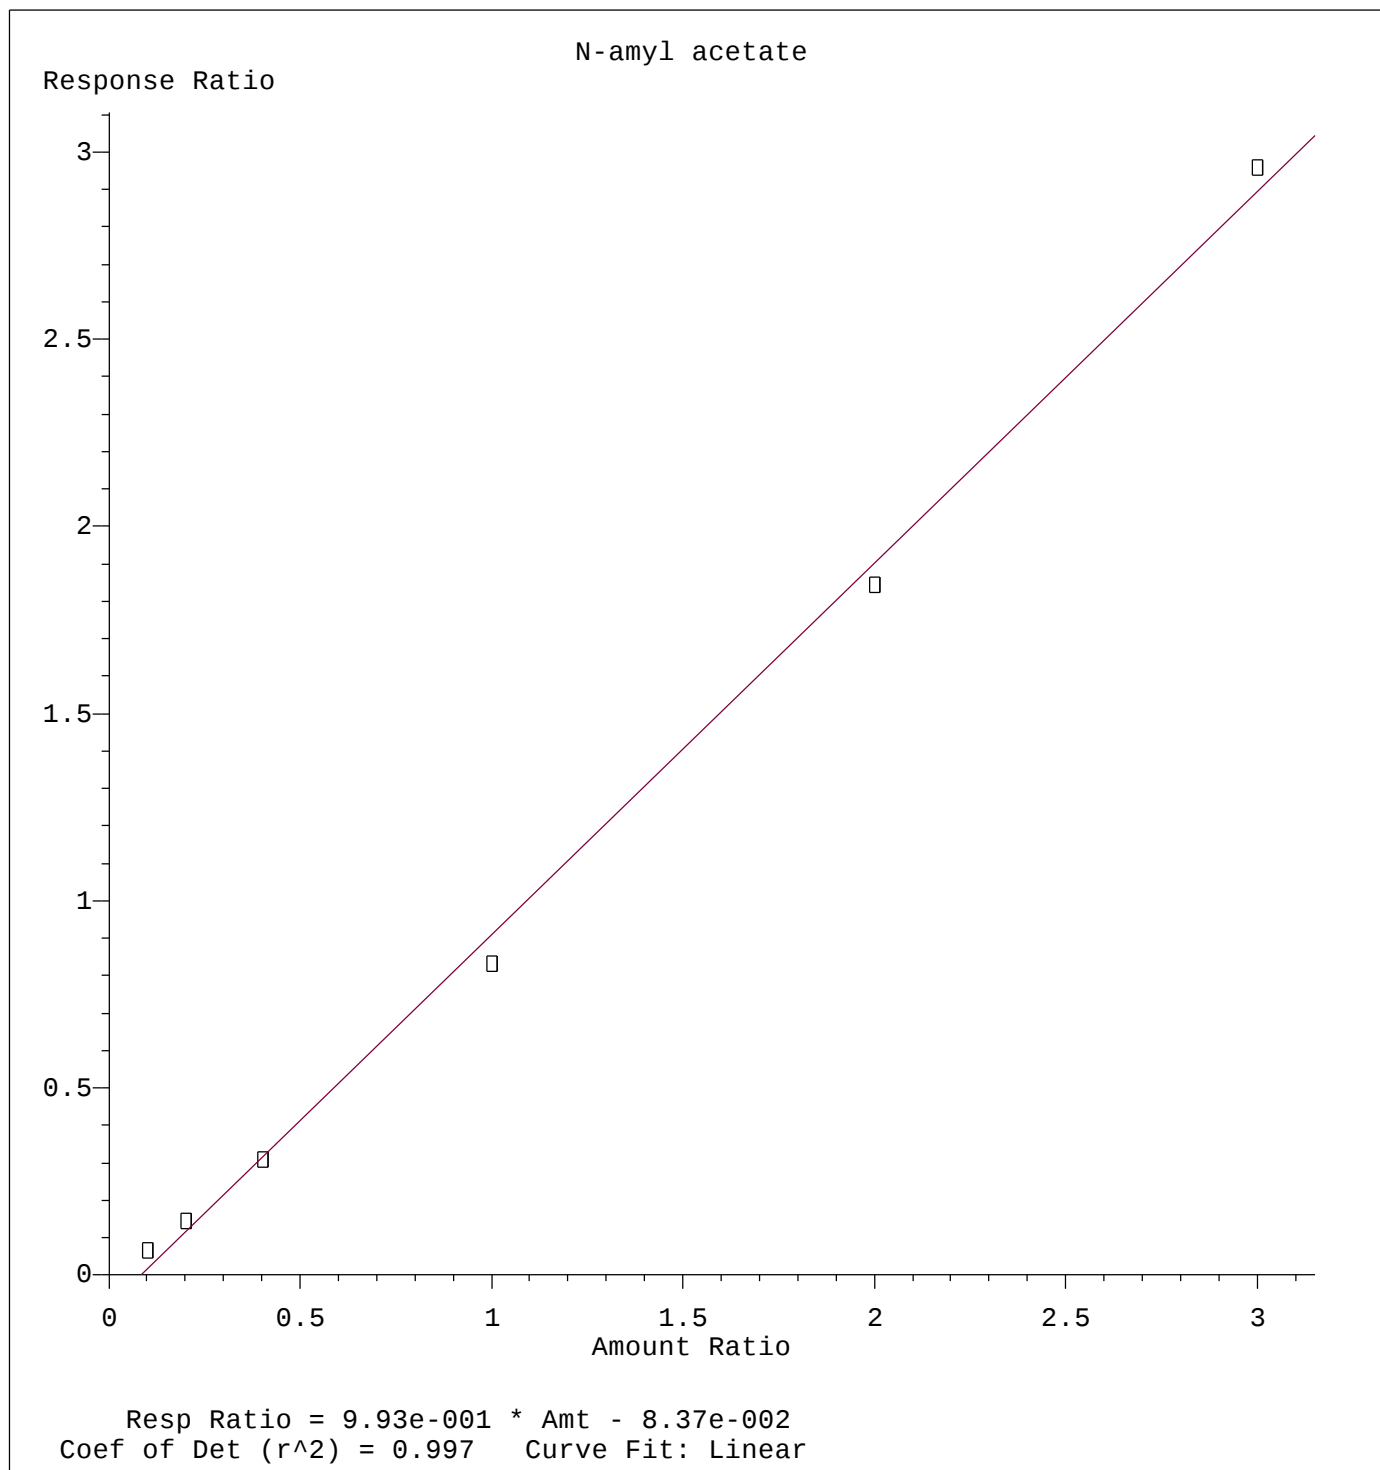

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030619S.M
Calibration Table Last Updated: Thu Mar 07 07:22:06 2019

trans-1,4-Dichloro-2-butene

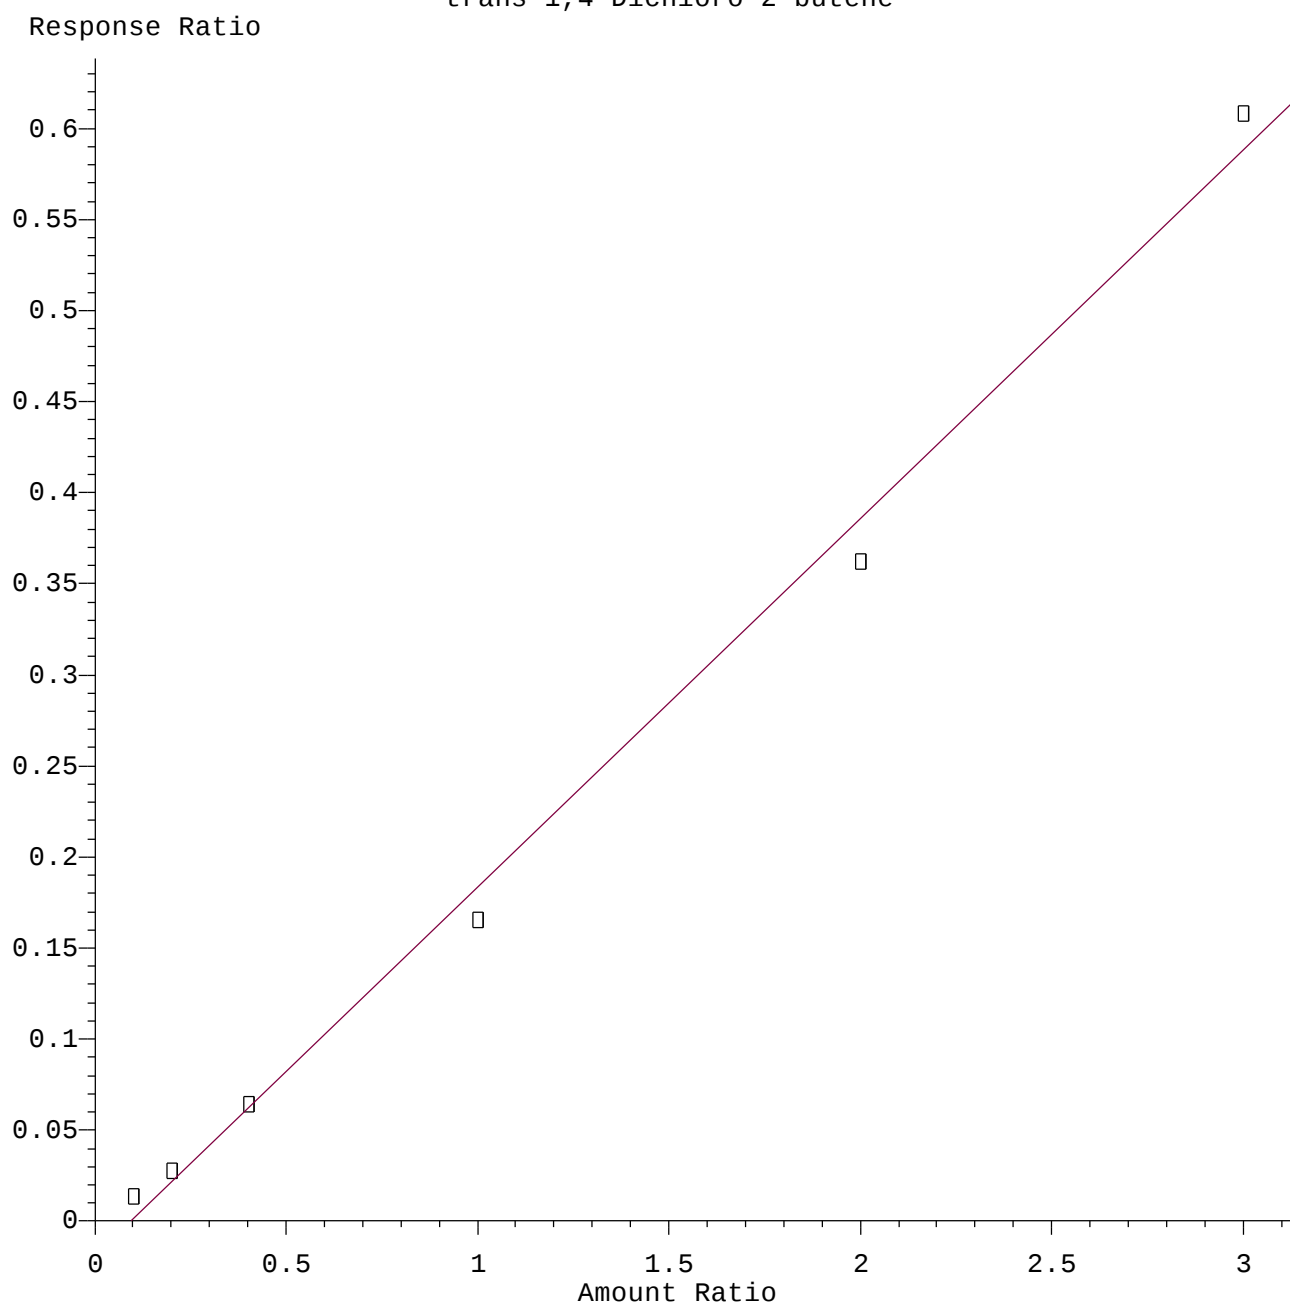

Resp Ratio = $2.02 \times 10^{-1} \times \text{Amt} - 1.92 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030619S.M
Calibration Table Last Updated: Thu Mar 07 07:22:06 2019