
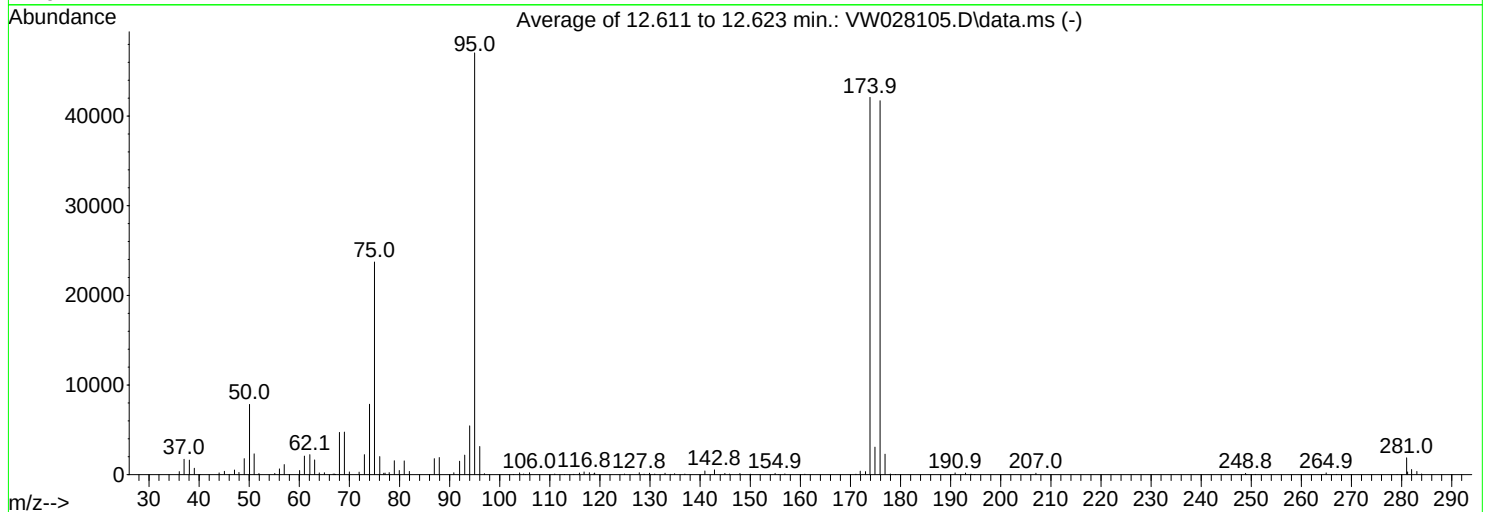


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030624\
Data File : VW028105.D
Acq On : 06 Mar 2024 08:30
Operator : SY/MD
Sample : BFB447
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB447

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Title : SFAM01.0
Last Update : Thu Mar 07 00:15:30 2024

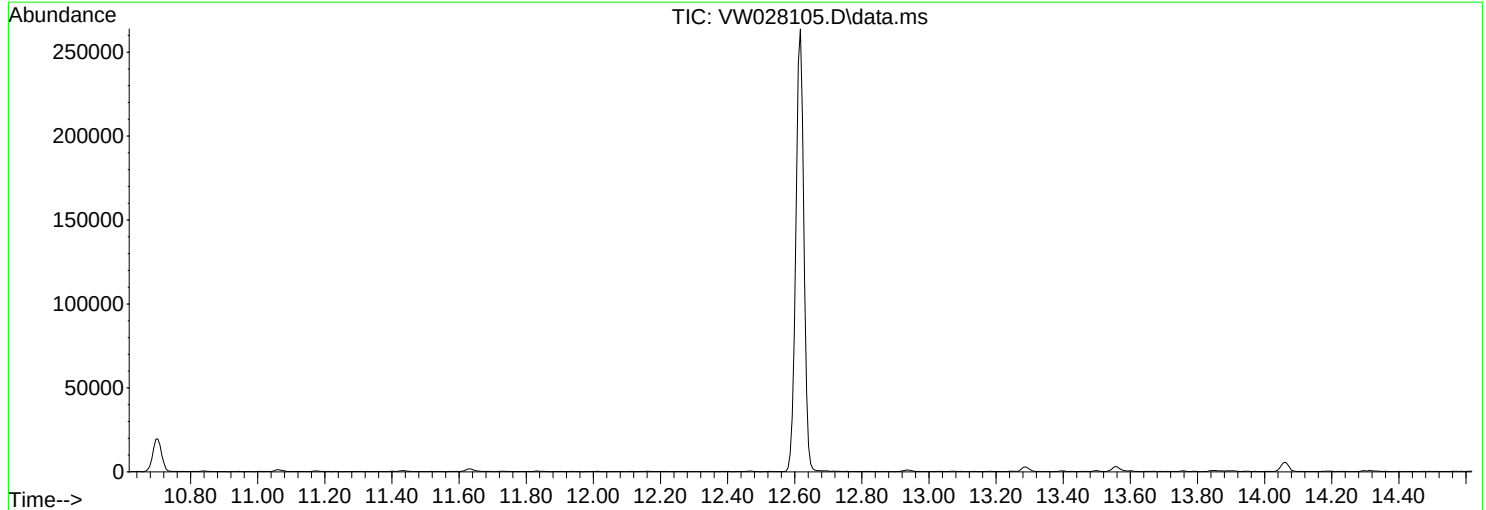

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	7841	PASS
75	95	30	80	50.4	23720	PASS
95	95	100	100	100.0	47056	PASS
96	95	5	9	6.7	3149	PASS
173	174	0.00	2	0.8	337	PASS
174	95	50	120	89.4	42088	PASS
175	174	5	9	7.3	3064	PASS
176	174	95	101	99.1	41712	PASS
177	176	5	9	5.5	2282	PASS

m/z	Abundance
40.00	139.0
44.00	89.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.00	415.0
37.00	1880.0
38.10	1745.0
39.10	768.0
40.10	134.0
44.00	353.0
45.10	446.0
46.00	93.0
47.00	424.0
47.90	268.0
49.00	1935.0
50.00	8453.0
51.00	2457.0
52.00	117.0
55.10	133.0
56.00	745.0
57.00	1338.0
58.00	72.0
60.10	561.0
61.00	2276.0
62.10	2505.0
63.00	1700.0
64.00	198.0
65.00	207.0
67.00	214.0
68.00	5107.0
69.00	4908.0
70.00	333.0
72.00	278.0
73.00	2329.0
74.00	8169.0
75.00	24848.0
76.10	2098.0
76.80	262.0
77.20	214.0
78.00	213.0
78.90	1754.0
79.90	580.0
80.90	1609.0
82.00	353.0
87.00	2000.0
88.00	2044.0
90.90	242.0
92.00	1502.0
93.00	2224.0
94.00	5457.0
95.00	49160.0
96.00	3198.0
97.00	83.0
102.80	77.0
104.00	191.0
104.80	104.0
105.90	219.0
111.00	80.0
112.90	63.0
114.80	90.0
115.90	243.0
116.90	327.0
117.90	267.0
118.80	290.0
124.90	153.0
127.80	197.0
128.80	93.0
129.90	201.0
130.90	52.0
133.00	284.0
134.20	63.0
134.90	156.0
141.00	407.0
142.90	559.0
144.90	139.0
145.90	75.0
148.00	143.0
150.00	62.0
154.90	130.0
156.90	115.0
160.90	103.0
172.00	355.0
173.00	502.0
173.90	39336.0
174.90	3170.0
175.90	37272.0
176.90	2601.0
178.00	67.0
179.00	73.0
190.90	315.0
192.90	355.0
194.10	113.0
194.80	50.0
207.00	268.0
248.80	300.0
250.80	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

265.00	272.0
267.00	70.0
279.10	61.0
281.00	3322.0
282.10	760.0
283.10	637.0
284.00	141.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.10	283.0
37.00	2015.0
38.00	1945.0
39.00	786.0
40.10	167.0
44.10	282.0
45.10	431.0
47.00	678.0
48.00	286.0
49.00	1922.0
50.00	8777.0
51.00	2626.0
52.00	187.0
55.10	214.0
56.10	619.0
57.00	1233.0
60.00	483.0
61.00	2259.0
62.10	2584.0
63.00	1874.0
64.00	224.0
65.10	281.0
66.70	130.0
68.00	5062.0
69.00	5441.0
70.00	379.0
71.90	297.0
73.00	2485.0
74.00	9082.0
75.00	26344.0
76.00	2007.0
77.00	348.0
77.90	265.0
79.00	1680.0
79.90	448.0
80.90	1759.0
82.00	424.0
86.00	56.0
87.00	1896.0
87.90	2259.0
90.90	174.0
92.00	1715.0
93.00	2541.0
94.00	5928.0
95.00	50392.0
96.00	3508.0
96.90	108.0
103.80	260.0
104.80	105.0
106.00	247.0
111.00	88.0
115.90	190.0
116.80	253.0
117.90	227.0
119.00	267.0
124.90	74.0
127.80	188.0
128.80	83.0
129.90	162.0
131.00	87.0
133.00	179.0
134.00	50.0
134.90	98.0
137.00	92.0
140.90	510.0
142.90	645.0
145.00	181.0
145.90	77.0
147.90	120.0
150.00	80.0
154.90	144.0
156.90	73.0
160.90	64.0
171.10	71.0
172.00	502.0
173.90	46448.0
174.90	3350.0
175.90	47208.0
176.90	2422.0
177.90	98.0
190.90	145.0
193.00	127.0
194.00	61.0
207.00	135.0
248.90	141.0
264.90	230.0
267.00	57.0
281.00	2294.0
281.90	648.0
282.90	301.0
284.00	102.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.10	325.0
37.00	1265.0
38.00	1166.0
39.00	575.0
39.90	127.0
44.00	241.0
44.90	250.0
47.10	458.0
48.00	213.0
49.00	1479.0
50.10	6292.0
51.00	1885.0
51.80	84.0
55.00	90.0
56.10	559.0
57.10	788.0
60.00	328.0
61.00	1690.0
62.00	1591.0
63.10	1328.0
64.00	154.0
64.90	134.0
66.80	111.0
67.20	93.0
68.00	3986.0
69.00	3916.0
70.00	227.0
72.00	306.0
73.00	1879.0
74.00	6339.0
75.00	19968.0
76.00	1943.0
76.90	208.0
78.00	209.0
79.00	1249.0
80.00	379.0
81.00	1248.0
81.90	282.0
86.90	1471.0
88.00	1417.0
90.80	203.0
92.00	1306.0
93.00	1746.0
94.00	4966.0
95.00	41616.0
96.00	2742.0
97.00	118.0
104.00	164.0
105.20	63.0
106.00	191.0
111.00	59.0
115.80	117.0
116.90	331.0
117.90	151.0
118.90	289.0
127.90	248.0
129.90	129.0
131.00	94.0
134.90	86.0
136.90	117.0
140.90	331.0
142.80	405.0
144.90	117.0
145.80	91.0
148.00	131.0
155.00	157.0
155.70	52.0
156.90	59.0
171.10	75.0
171.90	309.0
173.00	510.0
173.90	40480.0
174.90	2671.0
175.90	40656.0
176.90	1823.0
177.90	61.0
190.90	130.0
192.90	71.0
207.00	71.0
249.10	99.0
265.00	85.0
281.20	887.0
281.90	305.0
283.00	138.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447