


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW030719\
 Data File : VW009030.D
 Acq On : 07 Mar 2019 09:55
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030719S.M
 Title : SW846 8260
 Last Update : Fri Mar 08 05:22:30 2019

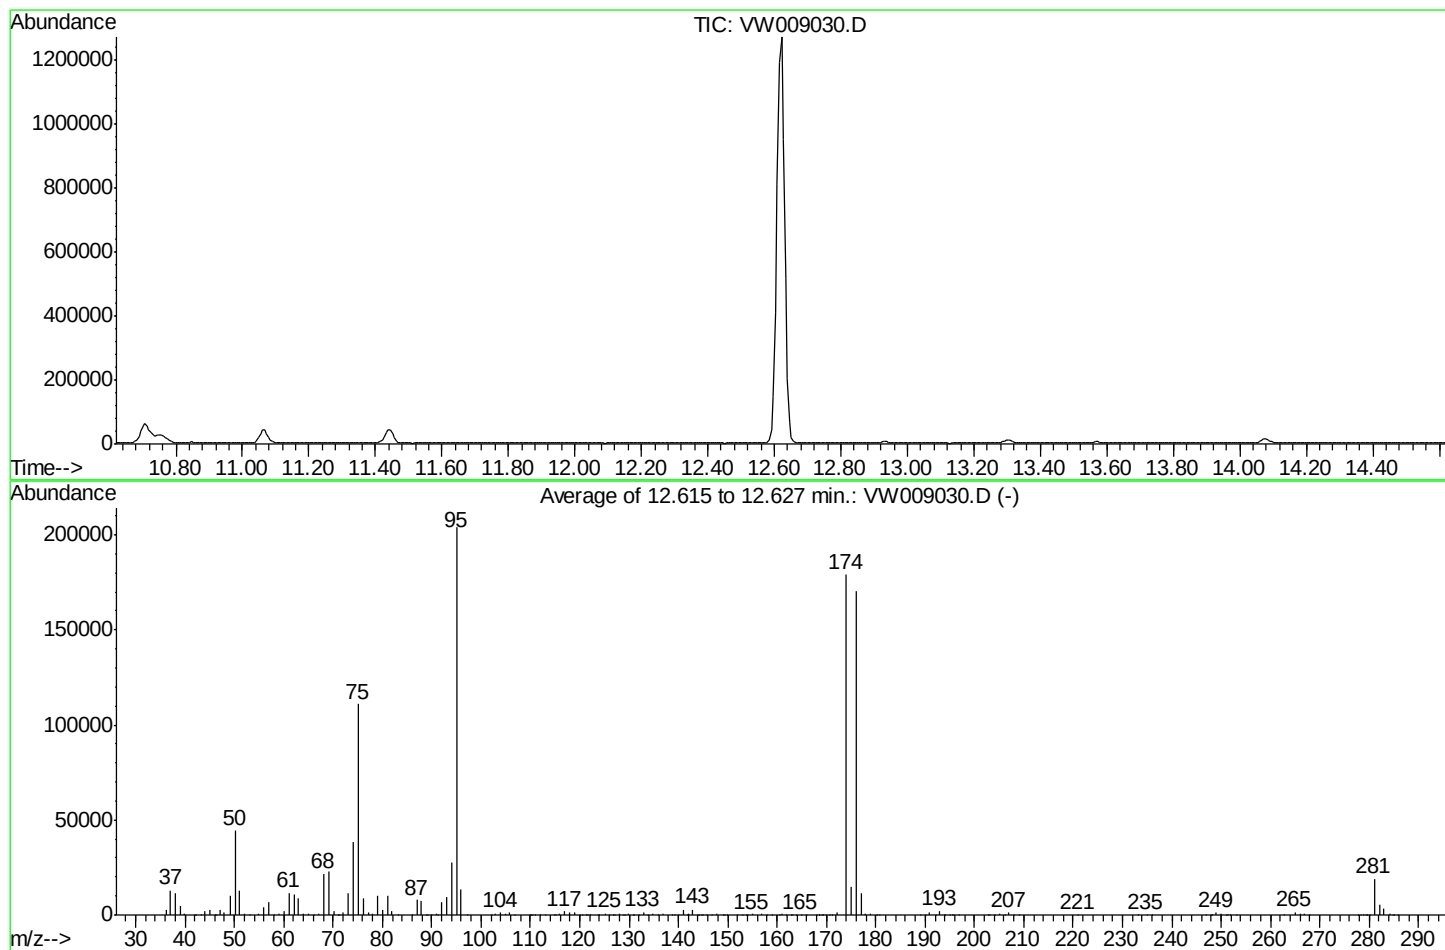

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	44240	PASS
75	95	30	60	54.5	111090	PASS
95	95	100	100	100.0	203989	PASS
96	95	5	9	6.7	13696	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.8	179093	PASS
175	174	5	9	8.2	14704	PASS
176	174	95	101	95.2	170560	PASS
177	176	5	9	6.7	11432	PASS