
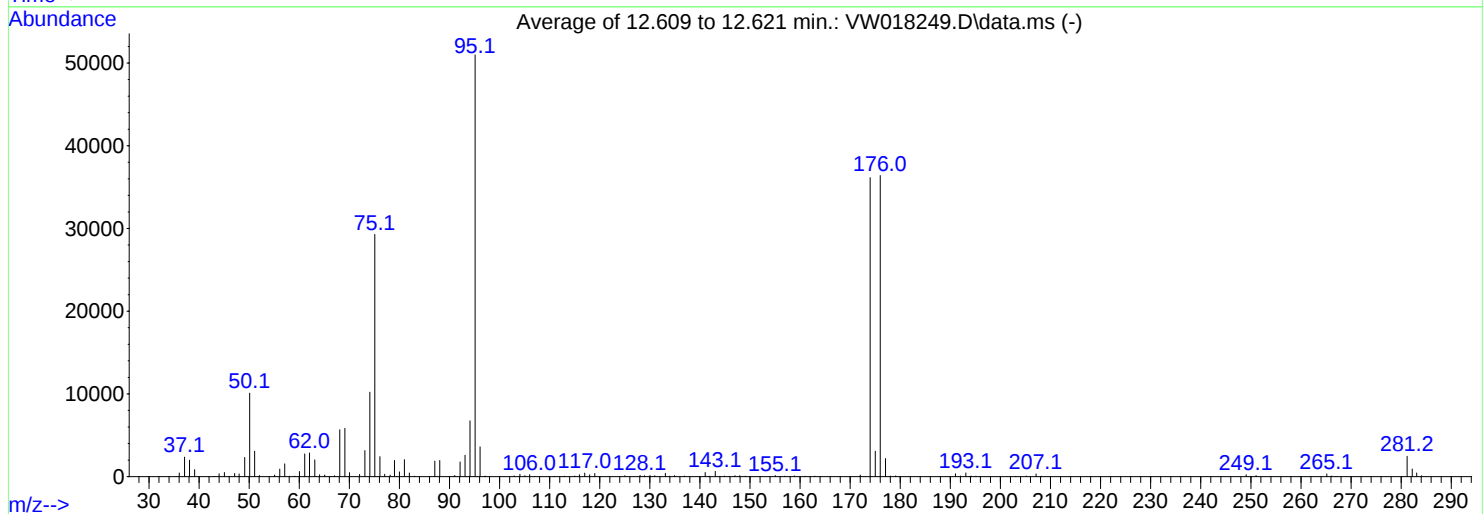


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030821\
 Data File : VW018249.D
 Acq On : 08 Mar 2021 11:15
 Operator : SY/VA
 Sample : BFB10
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB10

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Title : VOC Analysis
 Last Update : Tue Mar 09 00:50:17 2021

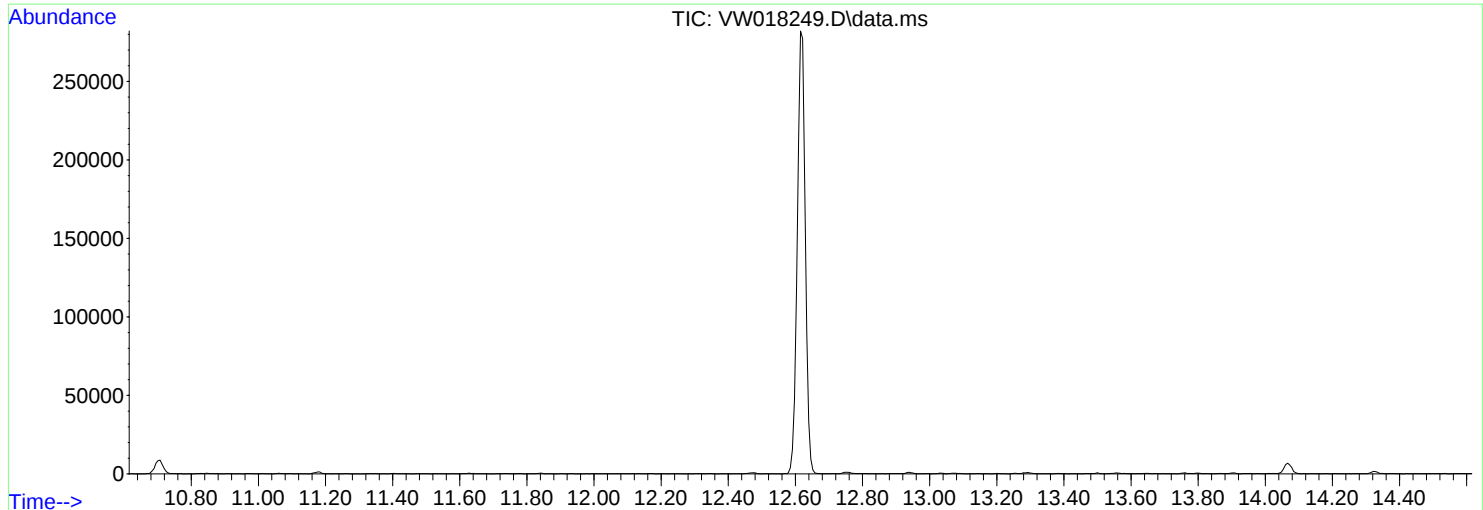

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	10106	PASS
75	95	30	80	57.4	29277	PASS
95	95	100	100	100.0	50989	PASS
96	95	5	9	7.0	3591	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.9	36157	PASS
175	174	5	9	8.5	3079	PASS
176	174	95	101	100.7	36400	PASS
177	176	5	9	6.0	2189	PASS

m/z	Abundance
36.00	351.0
37.10	2133.0
38.10	1515.0
39.10	854.0
44.00	361.0
45.00	478.0
47.10	329.0
48.00	267.0
49.10	1998.0
50.10	8340.0
51.10	2581.0
52.20	112.0
55.20	145.0
56.10	850.0
57.10	1257.0
59.20	110.0
60.10	676.0
61.10	2361.0
62.00	2586.0
63.10	1822.0
64.10	234.0
65.10	238.0
66.20	57.0
67.00	131.0
68.10	5055.0
69.10	5141.0
70.10	435.0
72.10	226.0
73.10	2799.0
74.10	8342.0
75.10	25048.0
76.10	2107.0
77.20	251.0
78.20	172.0
79.00	1763.0
80.00	486.0
81.00	1792.0
82.10	403.0
83.10	66.0
87.10	1664.0
88.10	1600.0
90.90	186.0
92.10	1403.0
93.10	2228.0
94.10	5574.0
95.10	42056.0
96.10	3117.0
97.00	117.0
102.90	121.0
104.00	255.0
105.00	86.0
106.00	232.0
107.00	57.0
111.00	88.0
115.10	78.0
115.90	265.0
117.00	391.0
118.10	139.0
119.00	302.0
125.00	182.0
128.00	148.0
129.00	103.0
129.90	217.0
131.00	90.0
133.10	766.0
134.00	122.0
135.00	86.0
136.90	107.0
141.10	417.0
143.00	548.0
144.90	77.0
147.00	91.0
147.90	87.0
149.10	95.0
150.00	51.0
155.10	135.0
156.90	58.0
158.80	66.0
161.00	94.0
163.00	75.0
172.00	142.0
174.00	27656.0
175.00	2223.0
176.00	26120.0
177.00	1827.0
178.00	170.0
179.10	187.0
180.10	97.0
191.00	482.0
192.00	107.0
193.10	655.0
194.20	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

195.10	133.0
203.10	78.0
205.20	85.0
207.10	422.0
208.10	97.0
249.00	238.0
250.00	60.0
251.10	180.0
265.20	408.0
266.20	135.0
281.20	2579.0
282.20	1338.0
283.10	637.0
284.10	141.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

m/z	Abundance
36.10	531.0
37.10	2536.0
38.10	2442.0
39.10	842.0
40.10	76.0
43.00	55.0
44.10	459.0
45.10	551.0
46.10	67.0
47.10	425.0
48.00	356.0
49.10	2532.0
50.10	11373.0
51.10	3391.0
52.00	132.0
55.10	261.0
56.10	883.0
57.10	1744.0
58.10	105.0
59.10	78.0
60.10	662.0
61.10	3186.0
62.10	2787.0
63.10	2176.0
64.00	272.0
65.10	187.0
67.10	110.0
68.10	6128.0
69.10	6341.0
70.10	619.0
72.10	333.0
73.10	3692.0
74.10	11364.0
75.10	32480.0
76.10	2722.0
77.00	377.0
78.20	191.0
79.00	2034.0
80.00	625.0
81.00	2137.0
81.90	444.0
83.00	67.0
87.00	2115.0
88.00	2162.0
91.10	207.0
92.10	2101.0
93.10	2936.0
94.10	7910.0
95.10	55720.0
96.10	4098.0
97.20	86.0
102.90	92.0
104.10	285.0
105.10	140.0
106.00	274.0
109.80	70.0
112.90	106.0
115.00	95.0
116.00	242.0
117.00	454.0
118.00	284.0
119.00	432.0
125.00	88.0
128.00	149.0
128.90	107.0
130.10	156.0
131.00	155.0
133.10	333.0
133.80	60.0
134.90	129.0
136.90	66.0
141.00	524.0
141.80	66.0
143.10	720.0
144.90	96.0
145.90	65.0
147.00	180.0
147.90	155.0
149.00	90.0
150.00	85.0
155.00	106.0
158.90	121.0
162.90	98.0
172.00	273.0
174.00	37160.0
175.00	3441.0
176.00	40400.0
177.00	2295.0
178.00	90.0
179.10	77.0
191.00	341.0
192.10	115.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

193.00	342.0
194.10	119.0
195.10	70.0
203.00	58.0
205.10	72.0
207.10	442.0
208.20	76.0
249.10	296.0
250.00	83.0
251.10	124.0
265.10	443.0
266.10	50.0
267.00	65.0
280.10	69.0
281.20	2965.0
282.20	930.0
283.10	408.0
284.10	170.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

m/z	Abundance
36.10	474.0
37.10	2402.0
38.10	2020.0
39.10	846.0
40.10	93.0
44.10	409.0
45.00	482.0
47.10	437.0
48.00	336.0
49.10	2460.0
50.10	10605.0
51.10	3282.0
52.00	165.0
55.00	155.0
56.10	969.0
57.10	1667.0
58.00	66.0
60.00	544.0
61.10	2706.0
62.10	3220.0
63.10	2080.0
64.10	206.0
65.10	177.0
67.10	126.0
68.10	5825.0
69.10	6026.0
70.00	383.0
72.00	253.0
73.10	2957.0
74.10	10932.0
75.10	30304.0
76.10	2453.0
77.00	257.0
78.10	220.0
79.00	2061.0
80.00	604.0
81.00	2198.0
82.00	518.0
83.00	62.0
87.10	1850.0
88.10	2125.0
91.00	212.0
92.10	1814.0
93.10	2615.0
94.10	6751.0
95.10	55192.0
96.10	3557.0
97.20	96.0
102.90	63.0
104.00	351.0
105.00	129.0
106.00	256.0
110.90	58.0
112.90	51.0
114.90	86.0
116.00	202.0
117.00	417.0
117.90	256.0
119.00	407.0
124.90	75.0
128.10	190.0
129.00	146.0
130.00	218.0
131.00	124.0
133.20	126.0
135.00	187.0
137.00	54.0
140.00	56.0
141.00	543.0
141.90	92.0
143.00	630.0
144.00	72.0
144.90	58.0
145.80	76.0
146.90	56.0
148.00	107.0
155.00	142.0
157.00	102.0
158.80	86.0
161.00	83.0
172.00	160.0
174.00	43656.0
175.00	3572.0
176.00	42680.0
177.10	2445.0
179.10	57.0
191.10	196.0
193.20	313.0
193.80	59.0
205.20	61.0
207.10	101.0
249.10	154.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

251.00	119.0
265.10	115.0
266.10	76.0
280.20	51.0
281.10	1848.0
282.20	537.0
283.20	262.0
284.00	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10

m/z	Abundance
40.00	129.0
44.00	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB10