



Methylene Chloride

Response Ratio

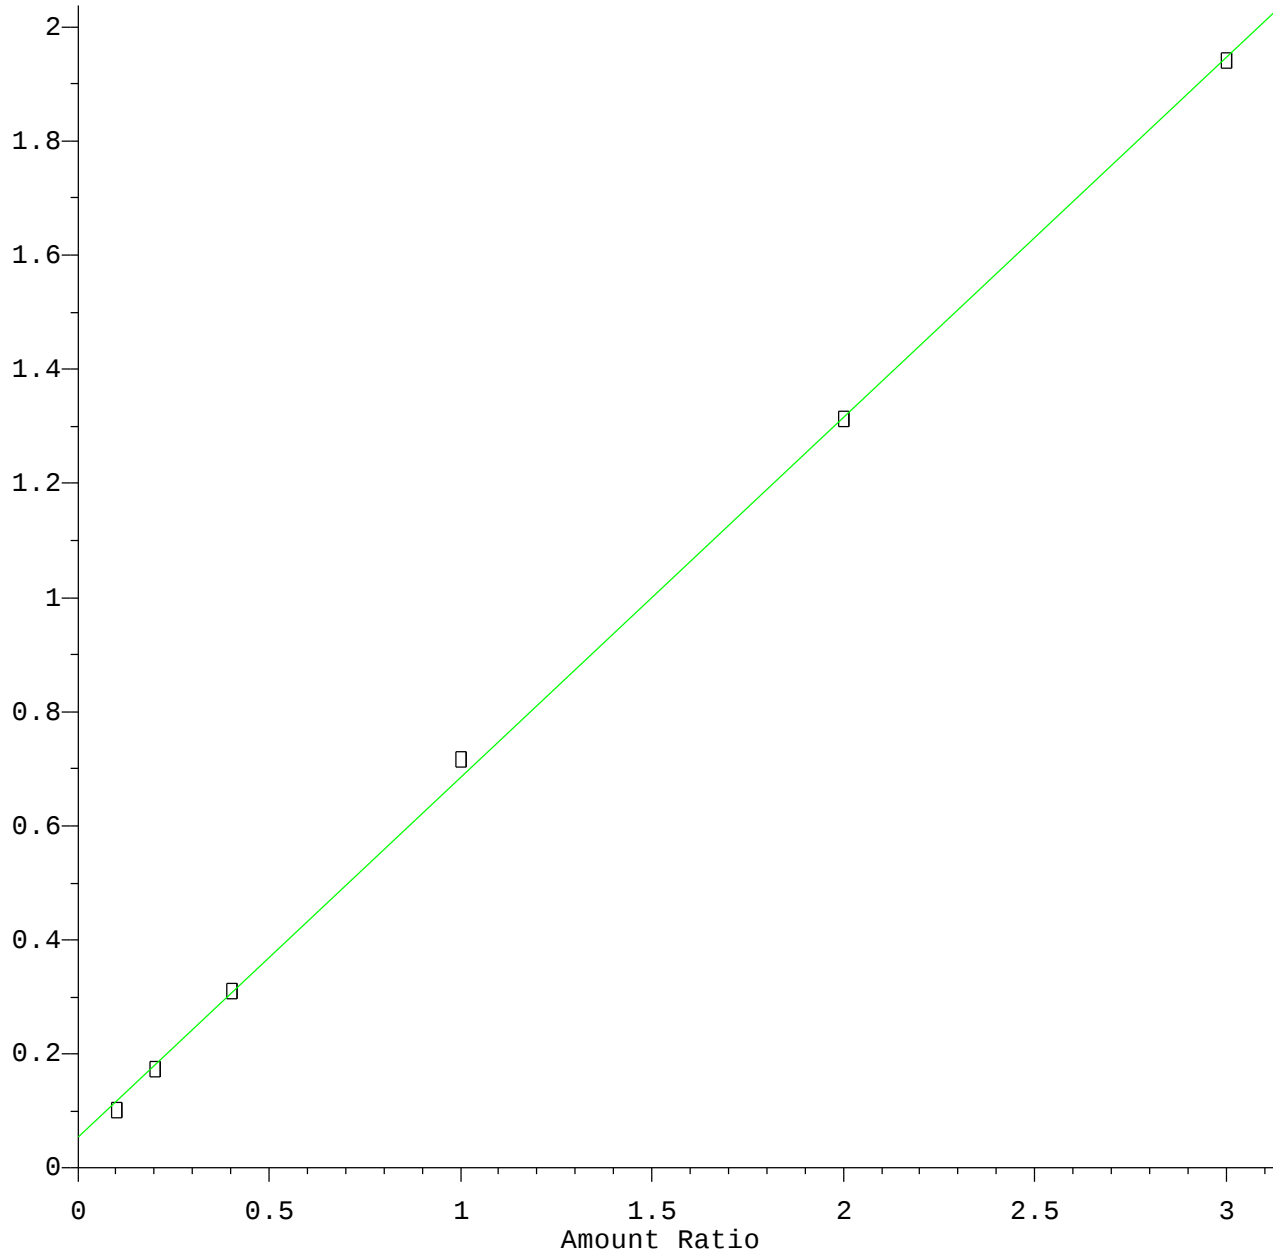


Resp Ratio = 6.31e-001 * Amt + 5.34e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030920S.M
Calibration Table Last Updated: Mon Mar 09 18:50:17 2020

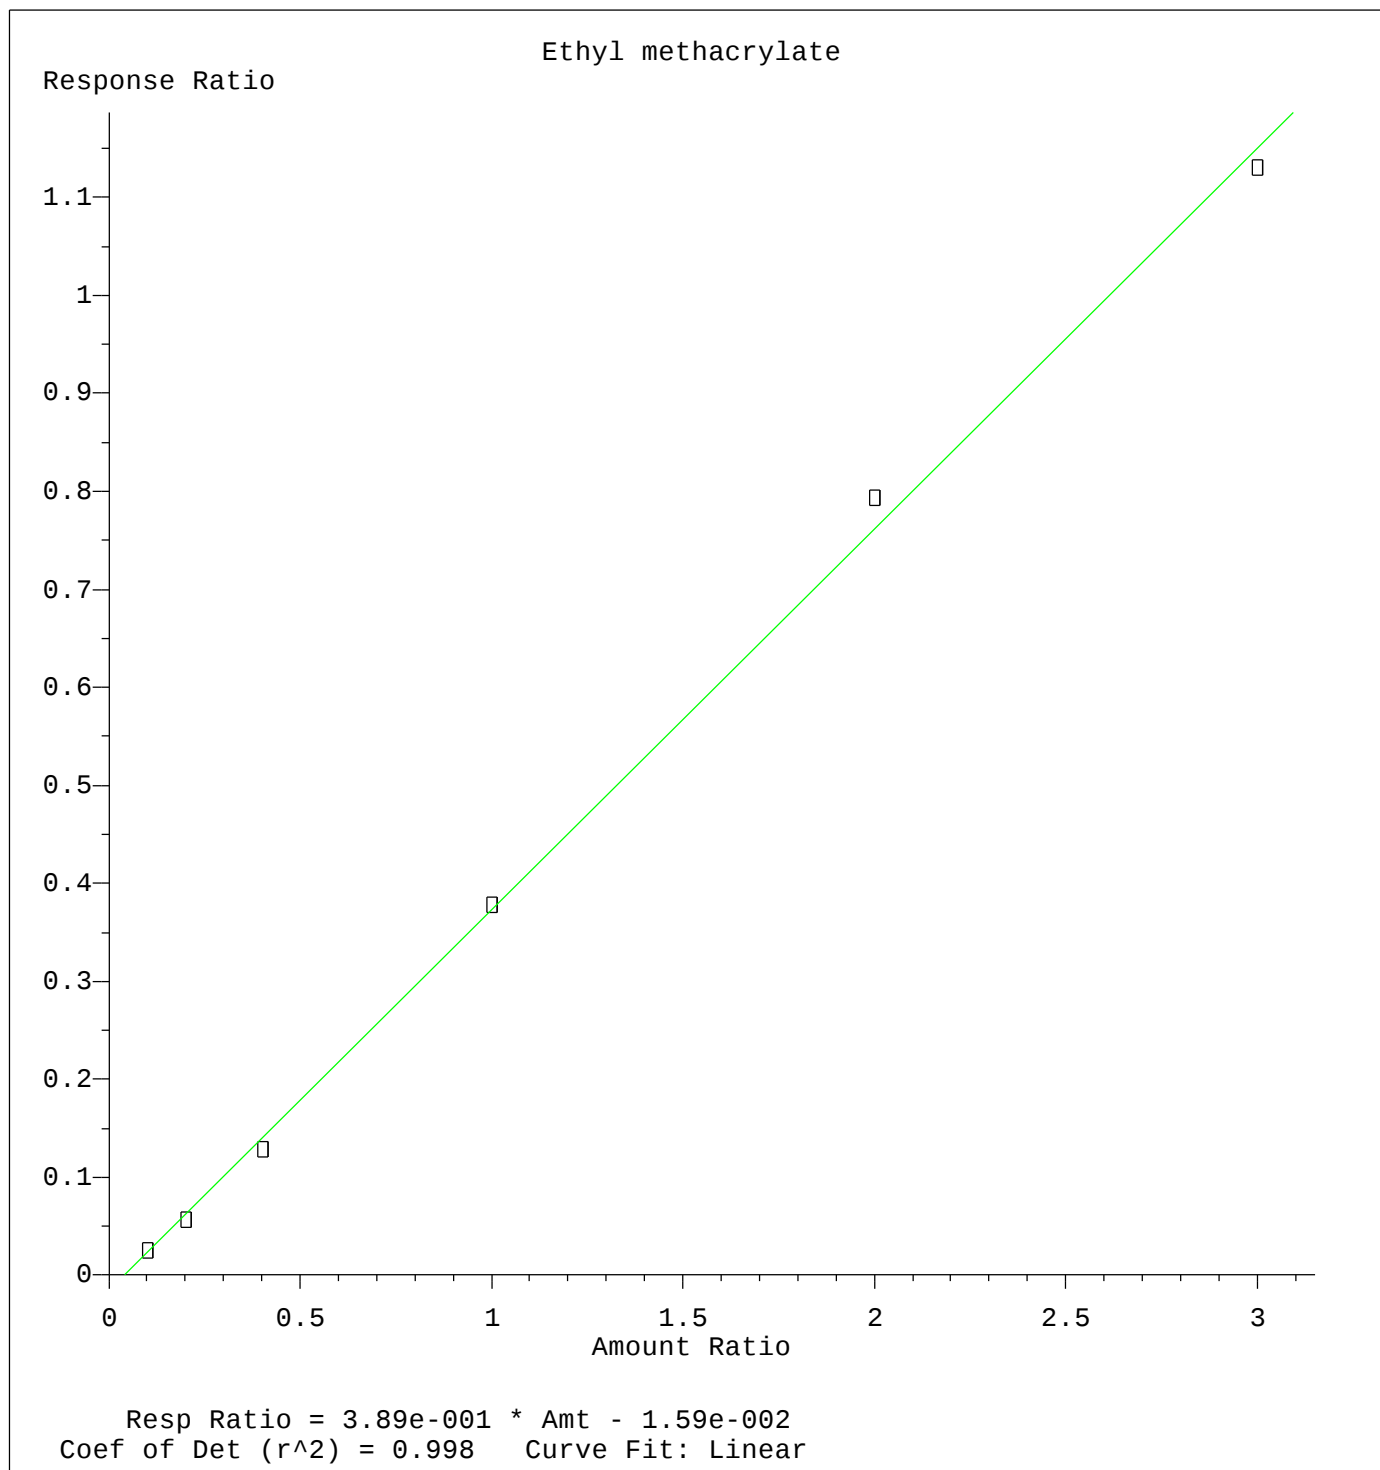


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030920S.M
Calibration Table Last Updated: Mon Mar 09 18:50:44 2020

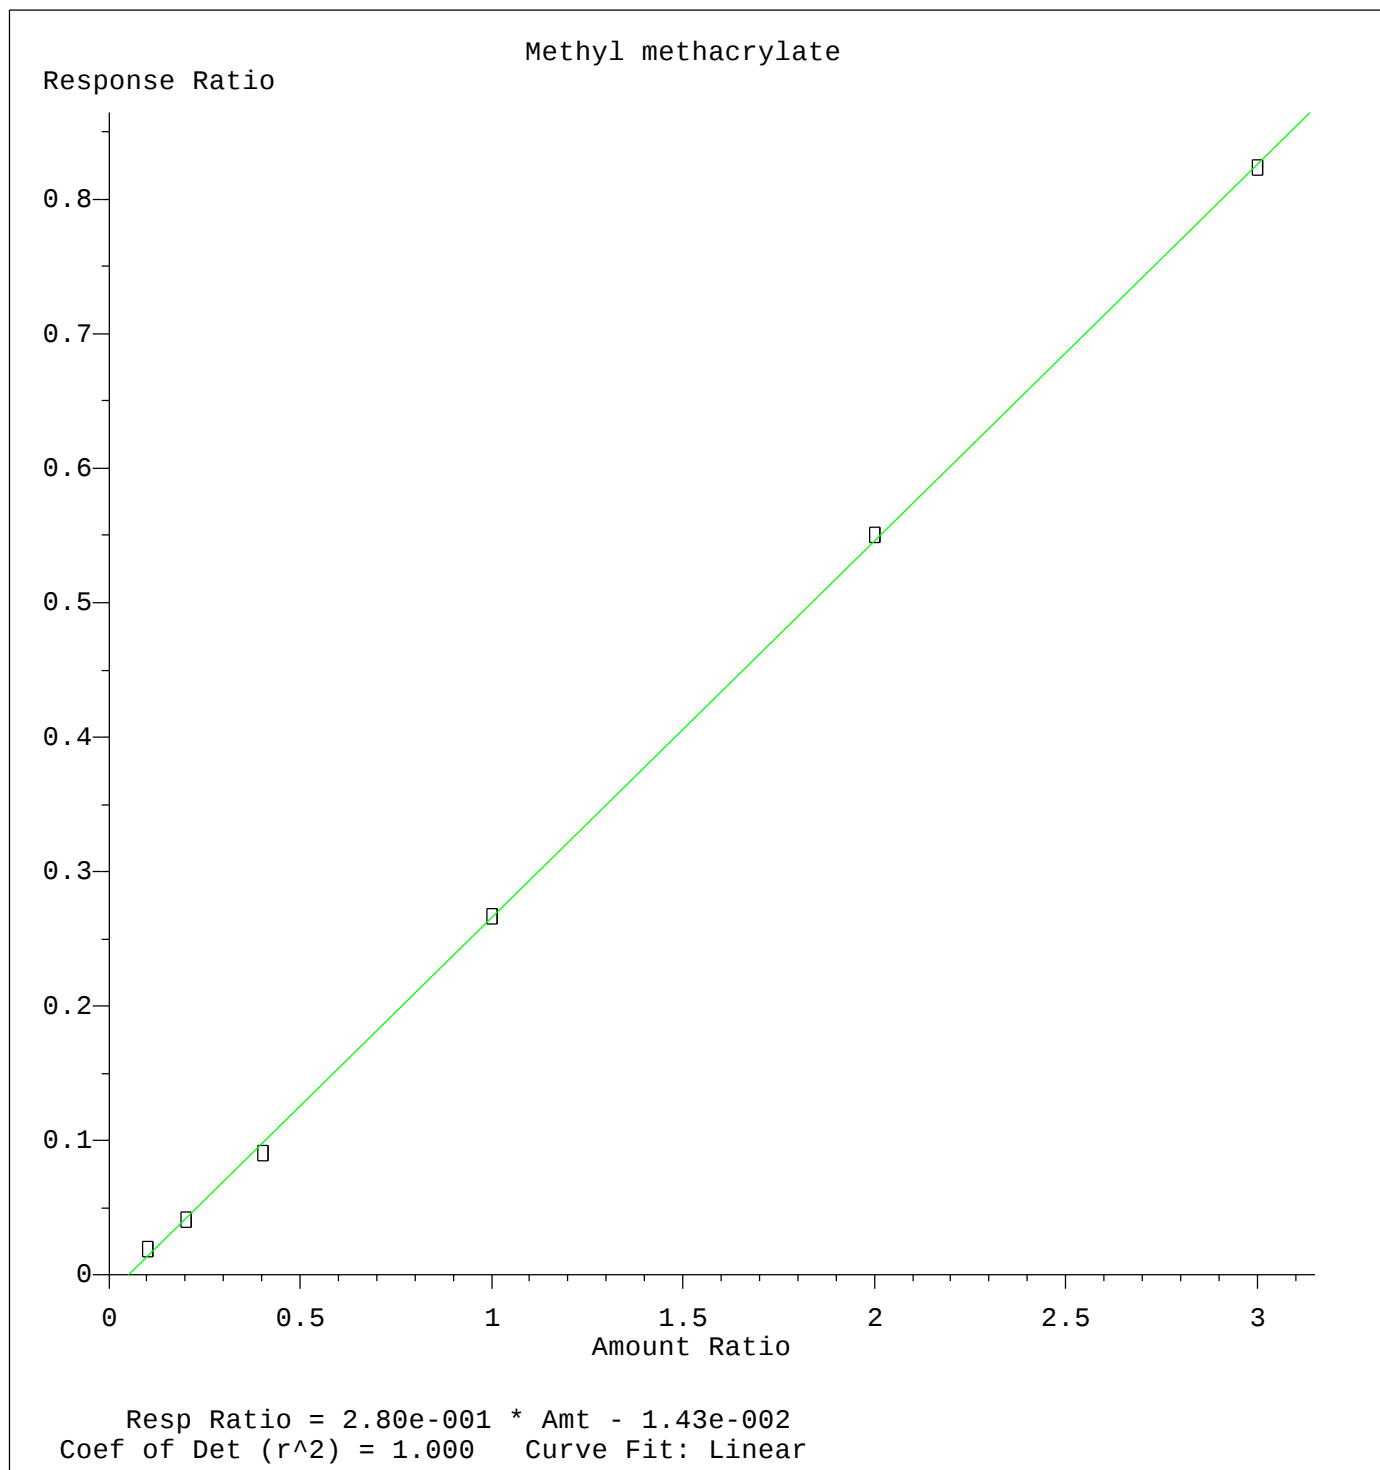

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030920S.M
Calibration Table Last Updated: Mon Mar 09 18:50:17 2020


Naphthalene

Response Ratio

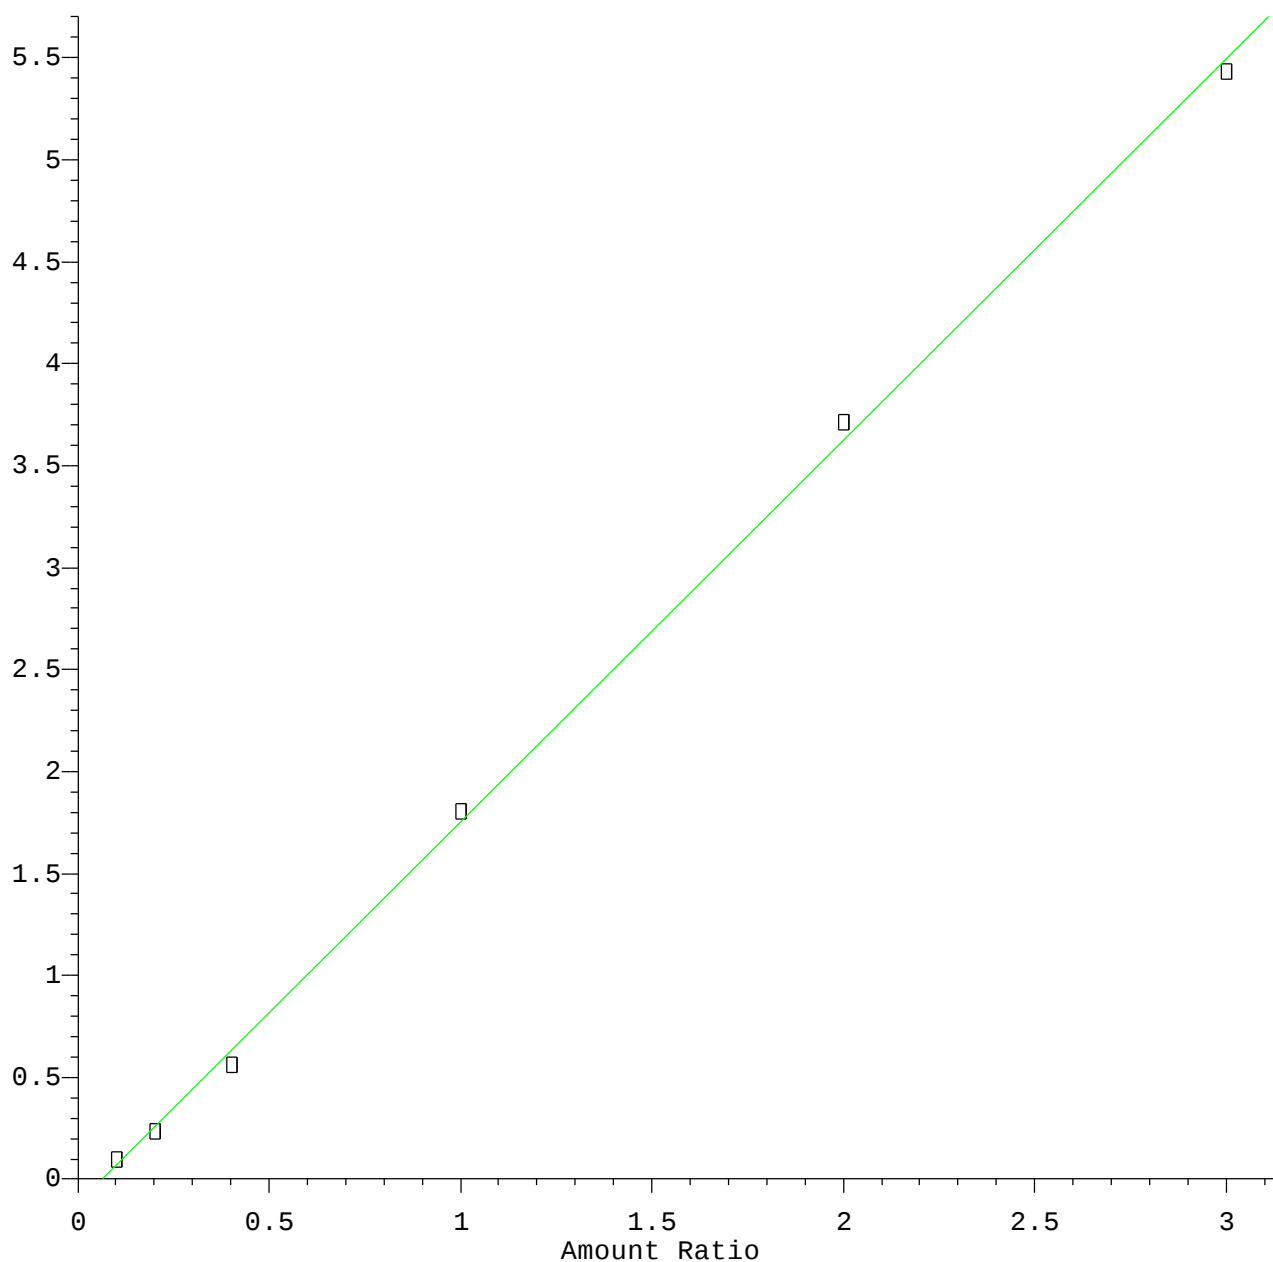

Resp Ratio = 1.87e+000 * Amt - 1.16e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030920S.M
Calibration Table Last Updated: Mon Mar 09 18:51:28 2020

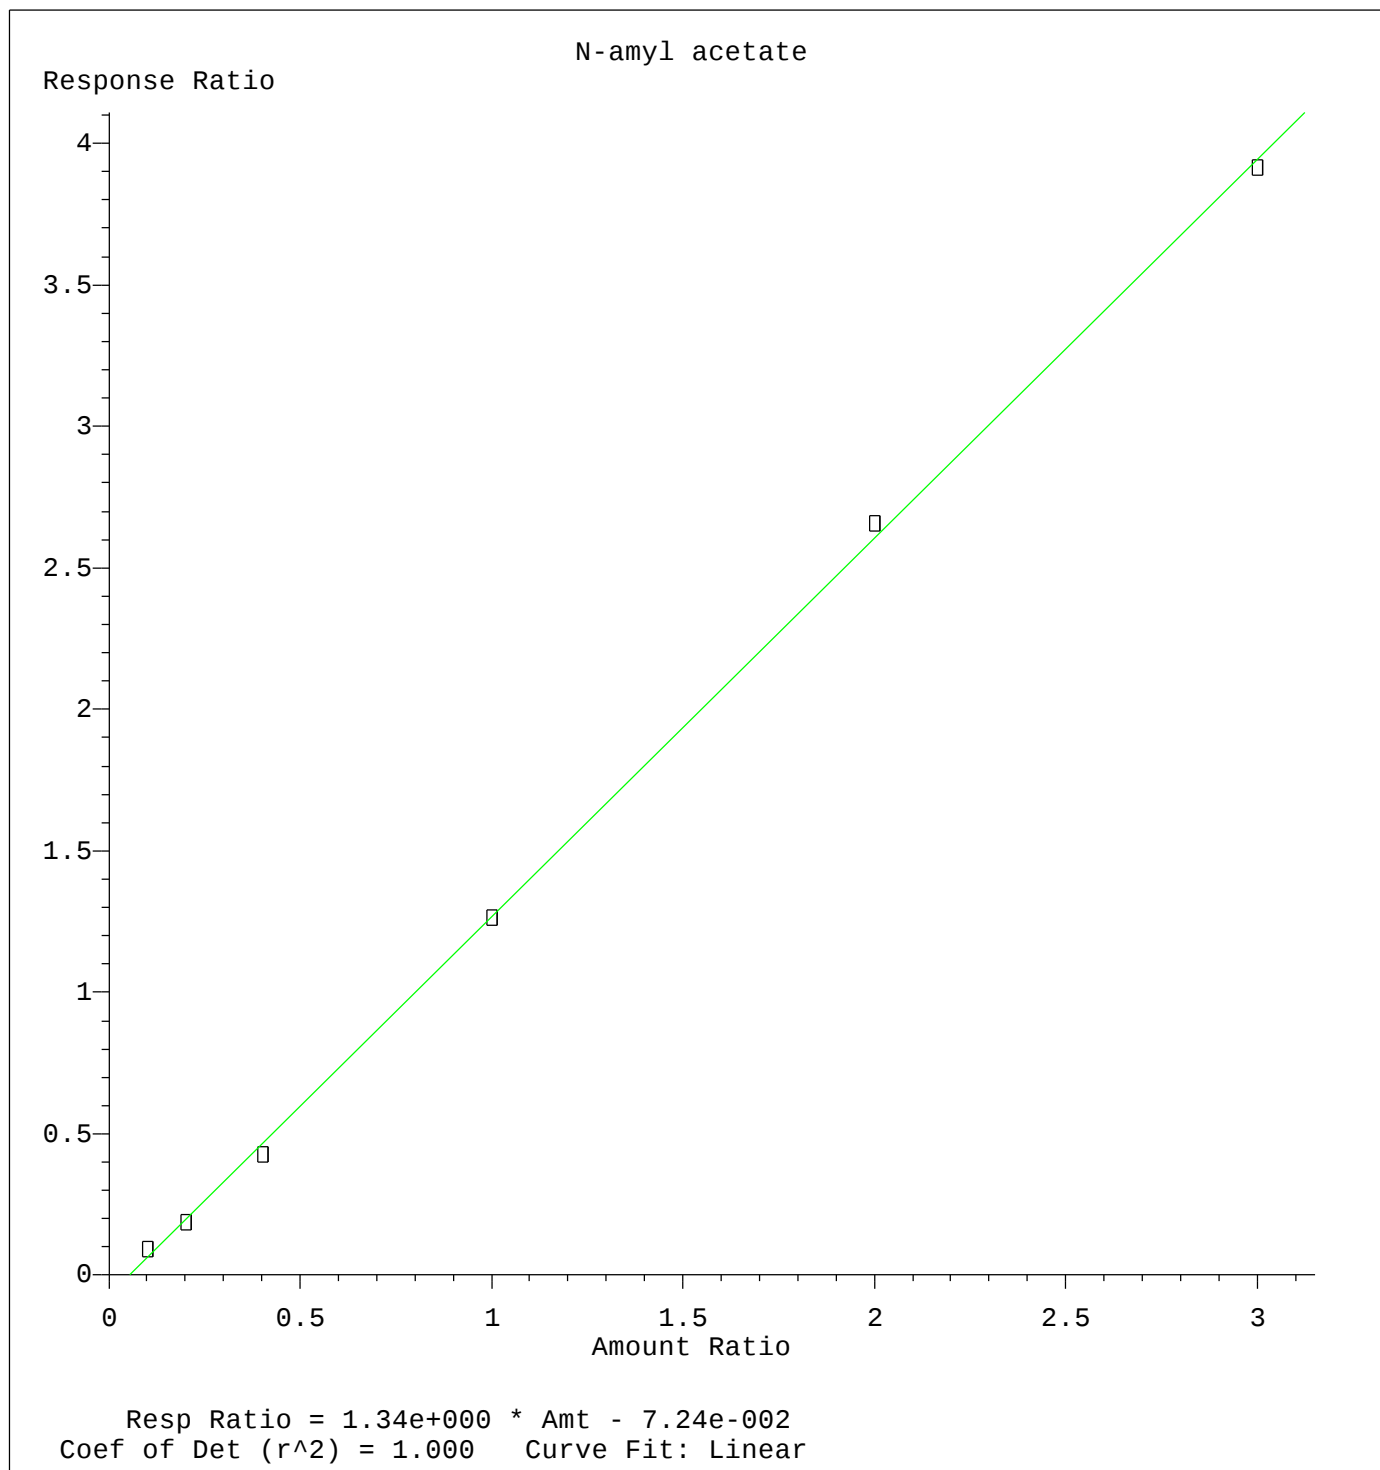

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030920S.M
Calibration Table Last Updated: Mon Mar 09 18:51:03 2020

2-Hexanone

Response Ratio

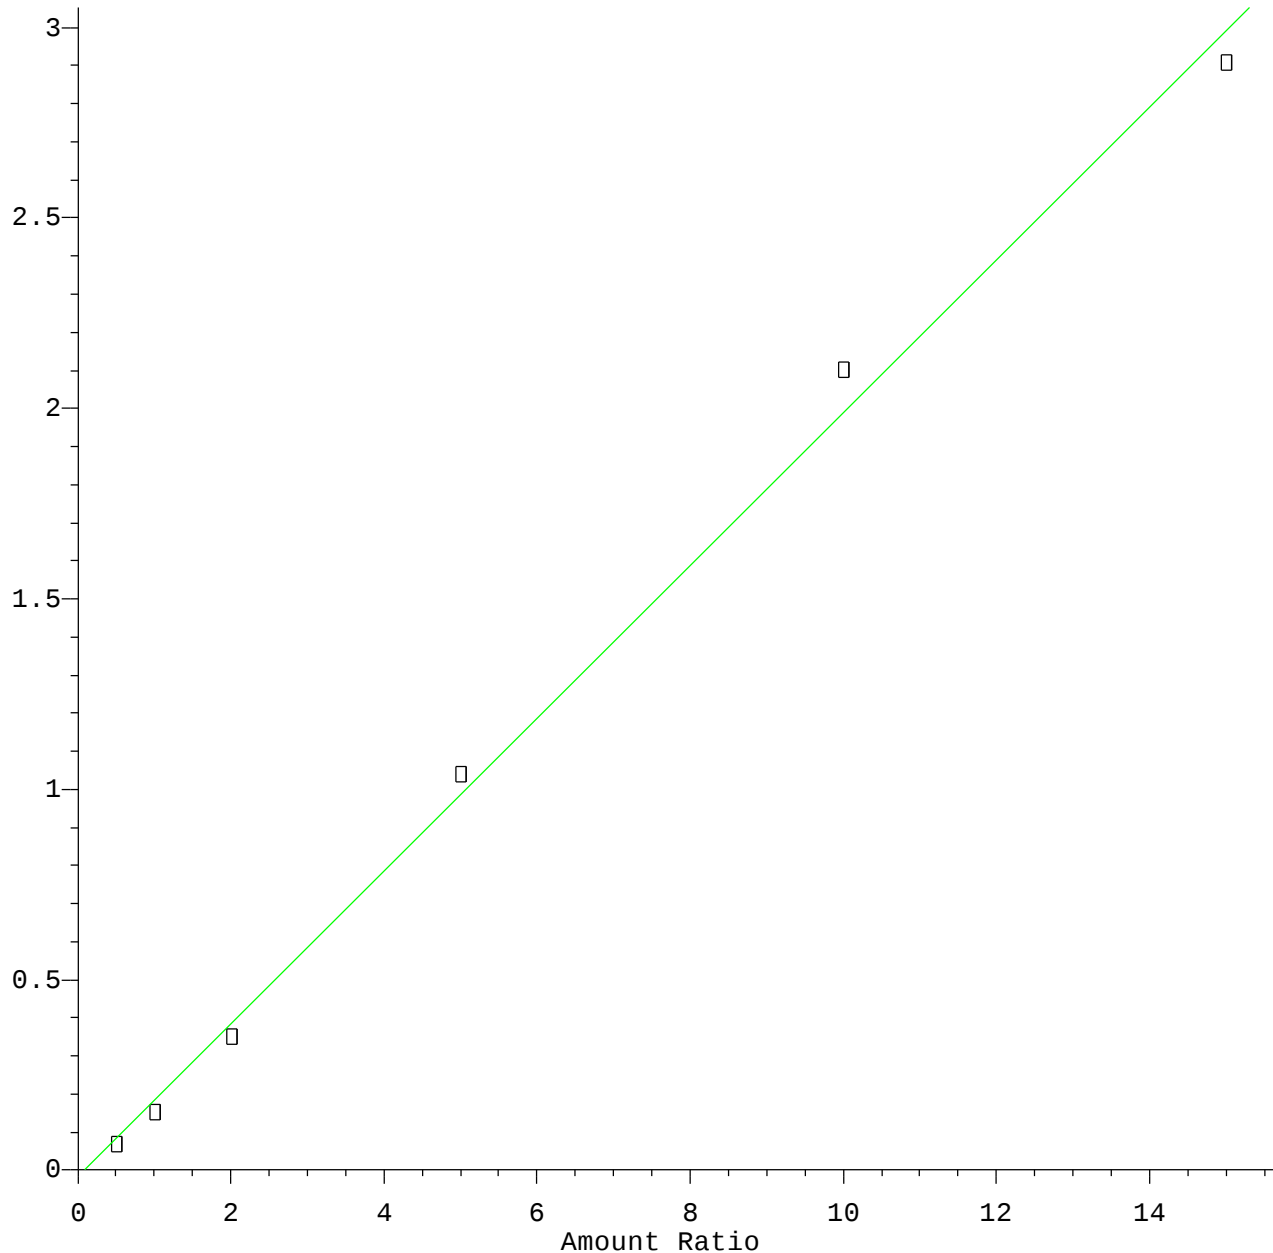

Resp Ratio = $2.01 \times 10^{-1} \times \text{Amt} - 1.87 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030920S.M
Calibration Table Last Updated: Mon Mar 09 18:51:03 2020