

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030921\
 Data File : VW018261.D
 Acq On : 09 Mar 2021 13:28
 Operator : SY/VA
 Sample : M1610-06
 Misc : 5.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG559

Manual Integrations
 APPROVED

MMDadoda
 3/12/2021 3:14:00 PM

Quant Time: Mar 10 02:14:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 10 02:13:53 2021
 Response via : Initial Calibration

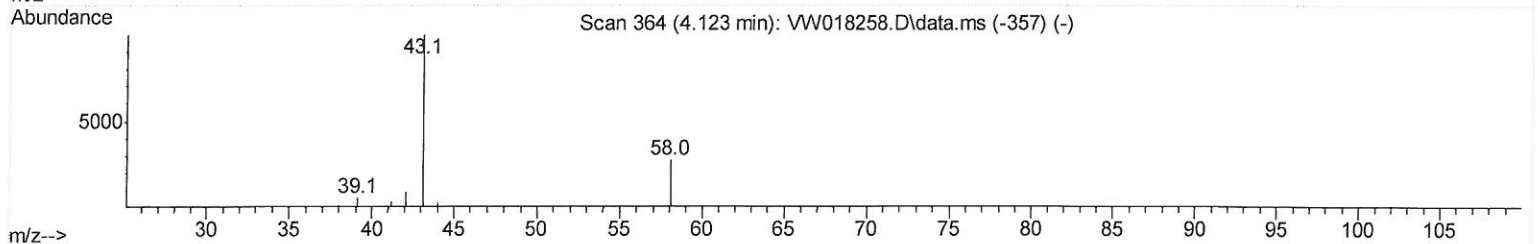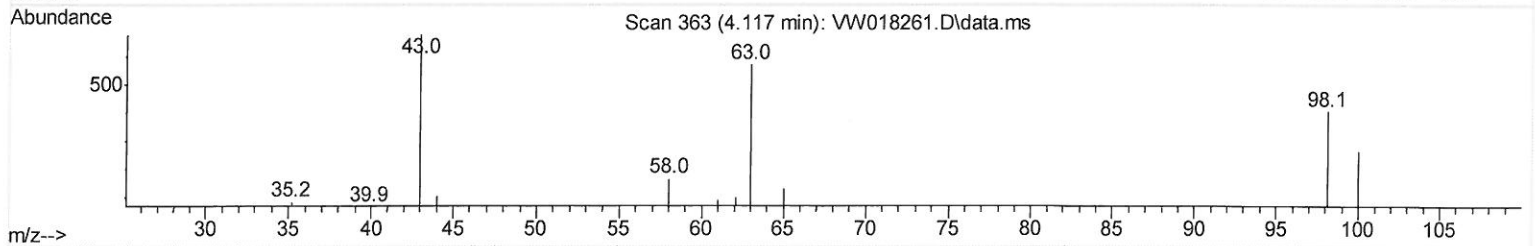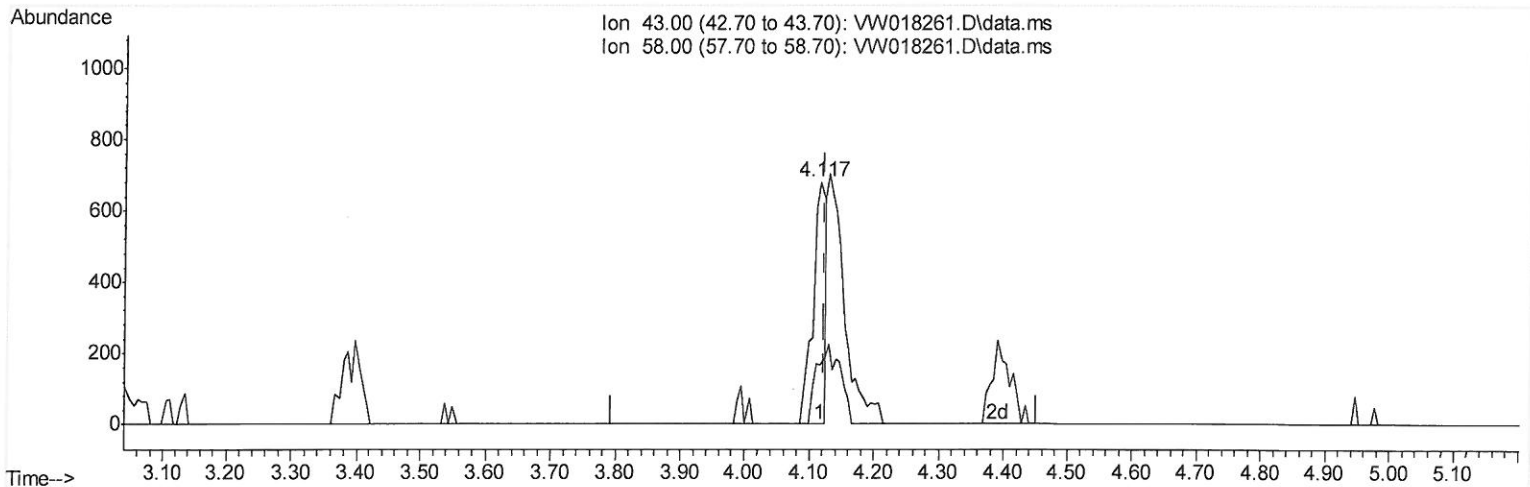

TIC: VW018261.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 1.56 ug/L

response 925

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	39.89
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030921\
 Data File : VW018261.D
 Acq On : 09 Mar 2021 13:28
 Operator : SY/VA
 Sample : M1610-06
 Misc : 5.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG559

Manual Integrations
 APPROVED

MMDadoda
 3/12/2021 3:14:00 PM

Quant Time: Mar 10 02:14:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 10 02:13:53 2021
 Response via : Initial Calibration

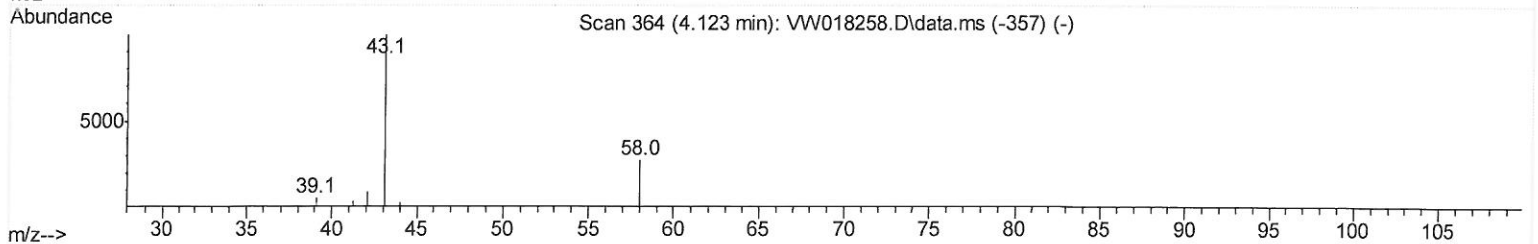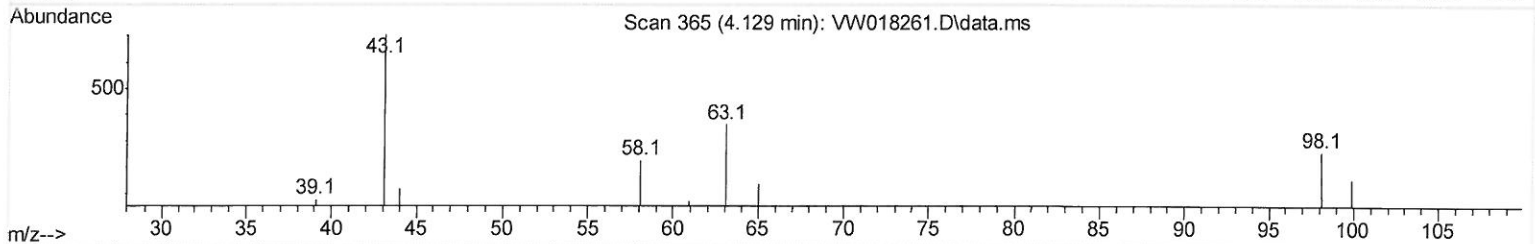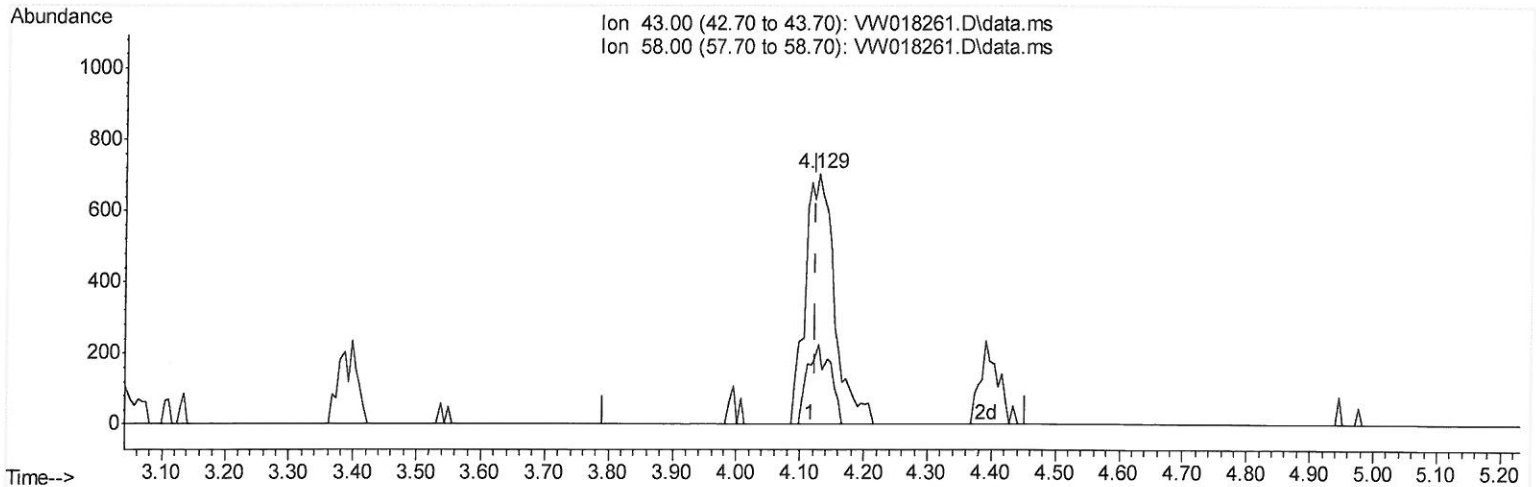

TIC: VW018261.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 3.76 ug/L m

03/18/21 Sy

response 2233

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	16.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030921\
 Data File : VW018261.D
 Acq On : 09 Mar 2021 13:28
 Operator : SY/VA
 Sample : M1610-06
 Misc : 5.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG559

Manual Integrations
 APPROVED

MMDadoda
 3/12/2021 3:14:00 PM

Quant Time: Mar 10 02:14:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 10 02:13:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	294968	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	254793	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	119636	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	97088	30.39	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	121.56%		
7) Chloroethane-d5	2.891	69	74370	28.67	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	114.68%		
10) 1,1-Dichloroethene-d2	4.025	63	154055	20.76	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	83.04%		
20) 2-Butanone-d5	7.074	46	34504	45.43	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	90.86%		
24) Chloroform-d	7.647	84	208811	26.13	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	104.52%		
26) 1,2-Dichloroethane-d4	8.305	65	115262	26.21	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	104.84%		
29) Benzene-d6	8.275	84	393600	29.02	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	116.08%		
33) 1,2-Dichloropropane-d6	9.274	67	104760	27.87	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	111.48%		
37) Toluene-d8	10.323	98	381311	29.13	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	116.52%		
38) trans-1,3-Dichloroprop...	10.579	79	49030	26.32	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	105.28%		
39) 2-Hexanone-d5	10.927	63	29090	46.53	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	93.06%		
48) 1,1,2,2-Tetrachloroeth...	12.688	84	77913	24.24	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	96.96%		
61) 1,2-Dichlorobenzene-d4	13.853	152	121054	27.84	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	111.36%		
Target Compounds						
13) Acetone	4.129	43	2233m	3.76	ug/L	Qvalue 97
16) Methylene chloride	4.921	84	8513	1.89	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030921\
Data File : VW018261.D
Acq On : 09 Mar 2021 13:28
Operator : SY/VA
Sample : M1610-06
Misc : 5.89G/10ML/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG559

Manual Integrations
APPROVED

MMDadoda
3/12/2021 3:14:00 PM

Quant Time: Mar 10 02:14:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 10 02:13:53 2021
Response via : Initial Calibration

