




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022247.D
 Acq On : 09 Mar 2022 12:44
 Operator : SY/VA
 Sample : N1818-18
 Misc : 5.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

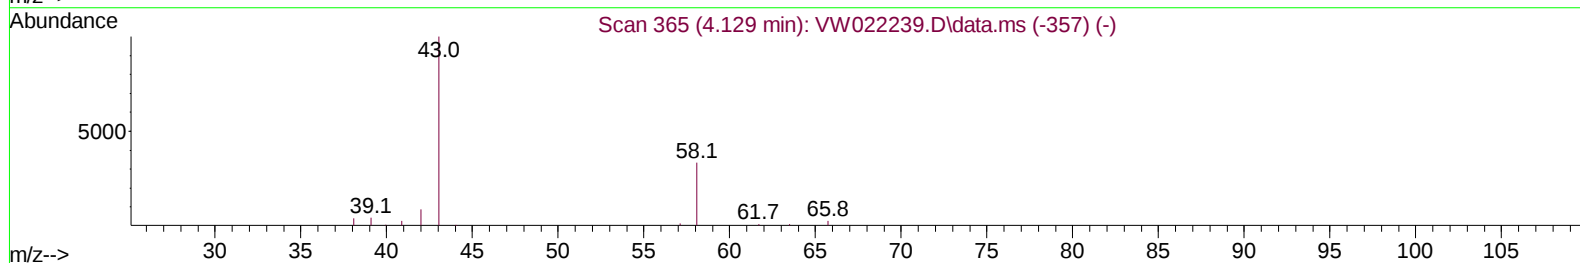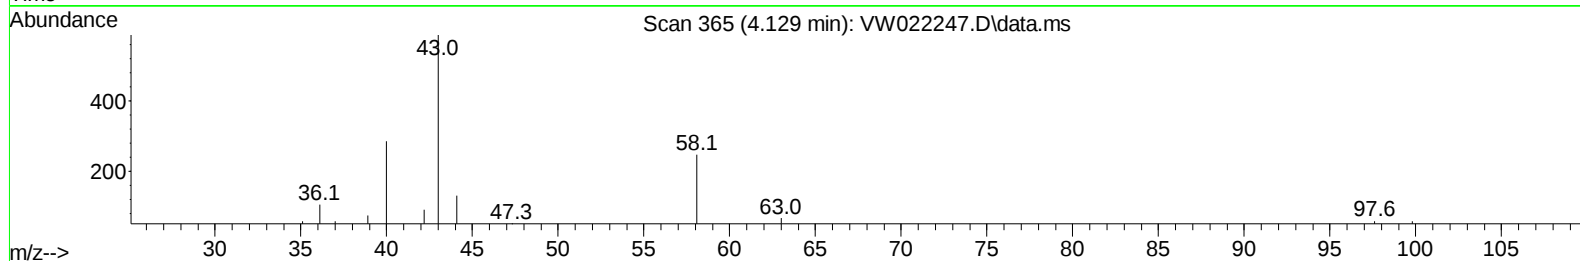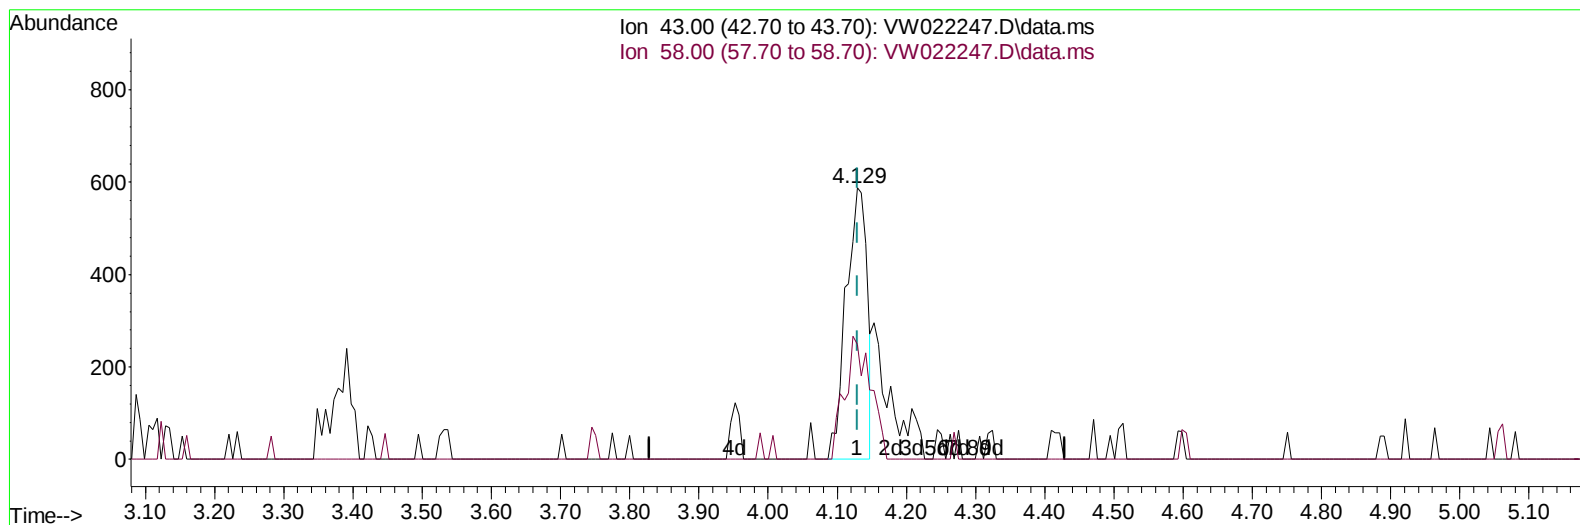

TIC: VW022247.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 3.61 ug/L

response 1243

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	45.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022247.D
Acq On : 09 Mar 2022 12:44
Operator : SY/VA
Sample : N1818-18
Misc : 5.98g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

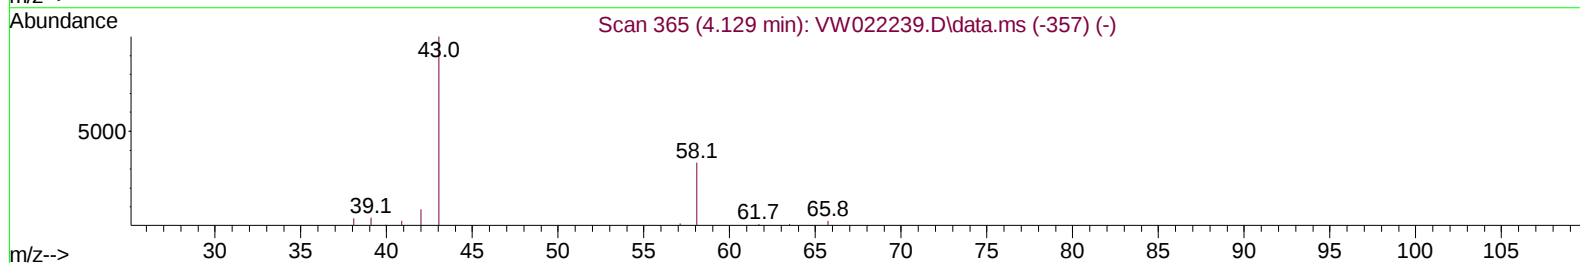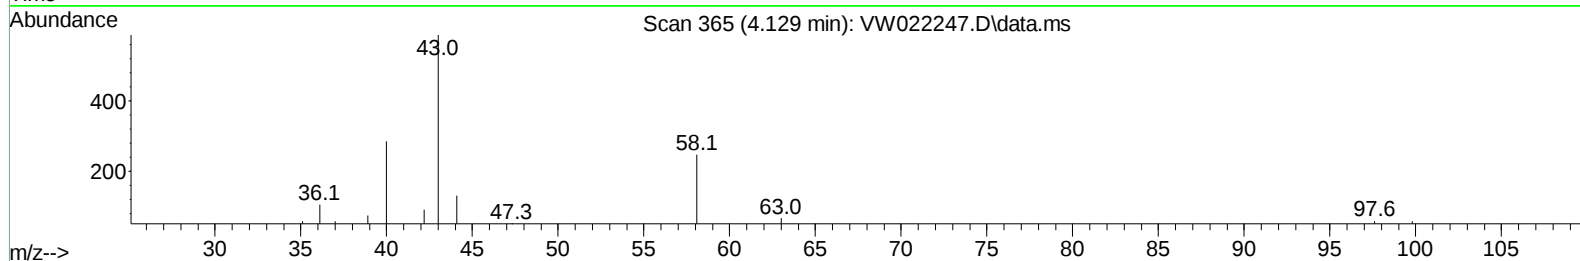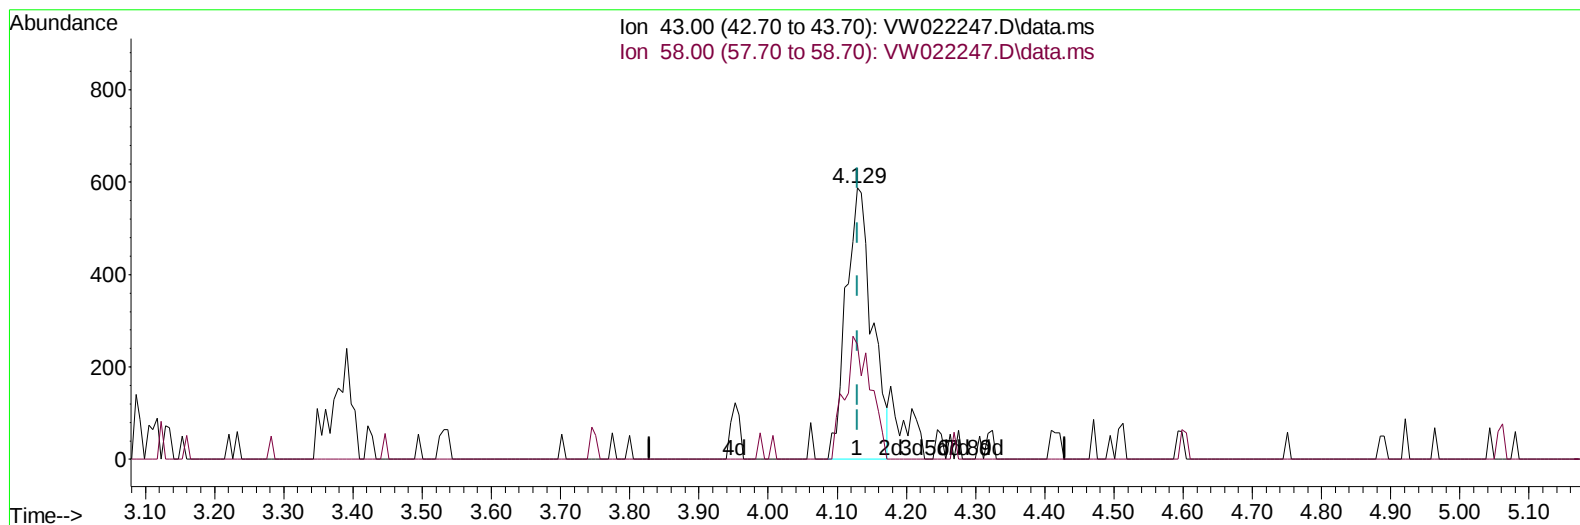

TIC: VW022247.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 4.45 ug/L m

response 1534

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	36.51
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022247.D
 Acq On : 09 Mar 2022 12:44
 Operator : SY/VA
 Sample : N1818-18
 Misc : 5.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		192363	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117		181373	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		89690	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		77630	30.941	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	123.760%	
7) Chloroethane-d5	2.879	69		49388	25.018	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	100.080%	
11) 1,1-Dichloroethene-d2	4.013	63		74560	19.405	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	77.640%	
21) 2-Butanone-d5	7.073	46		19903	47.180	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	94.360%	
24) Chloroform-d	7.646	84		110665	25.785	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	103.120%	
26) 1,2-Dichloroethane-d4	8.305	65		57793	25.905	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	103.600%	
32) Benzene-d6	8.274	84		221080	26.191	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	104.760%	
36) 1,2-Dichloropropane-d6	9.268	67		59479	25.373	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	101.480%	
41) Toluene-d8	10.323	98		216721	25.825	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	103.280%	
43) trans-1,3-Dichloroprop...	10.579	79		24898	23.955	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	95.800%	
47) 2-Hexanone-d5	10.920	63		17667	45.823	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	91.640%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		48658	23.652	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152		73930	25.663	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	102.640%	
Target Compounds							
13) Acetone	4.129	43		1534m	4.452	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022247.D
Acq On : 09 Mar 2022 12:44
Operator : SY/VA
Sample : N1818-18
Misc : 5.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:14:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

