




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022249.D
Acq On : 09 Mar 2022 13:32
Operator : SY/VA
Sample : N1818-13
Misc : 6.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF7

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

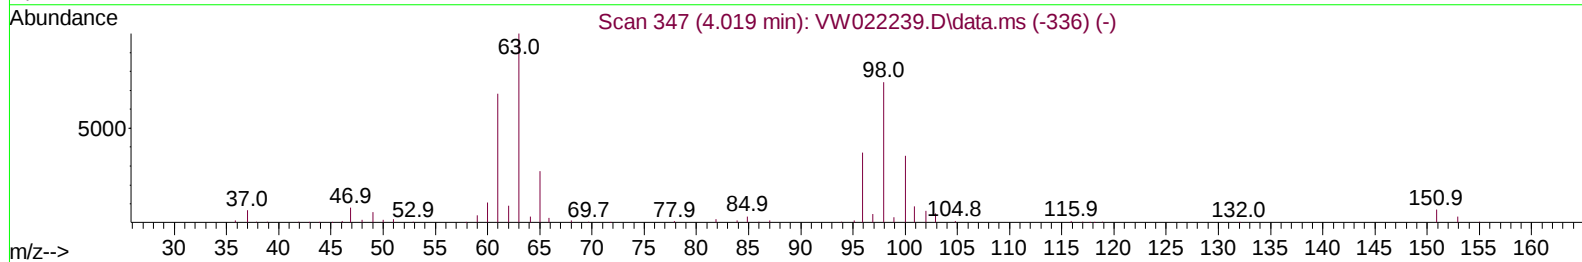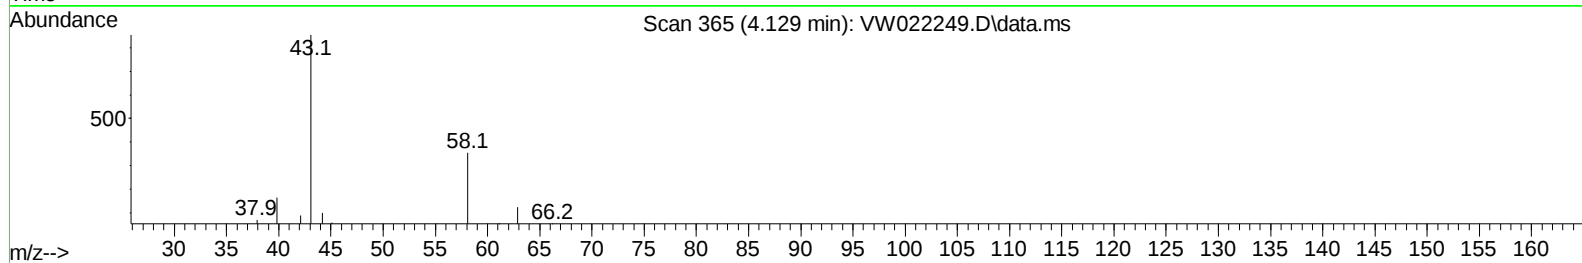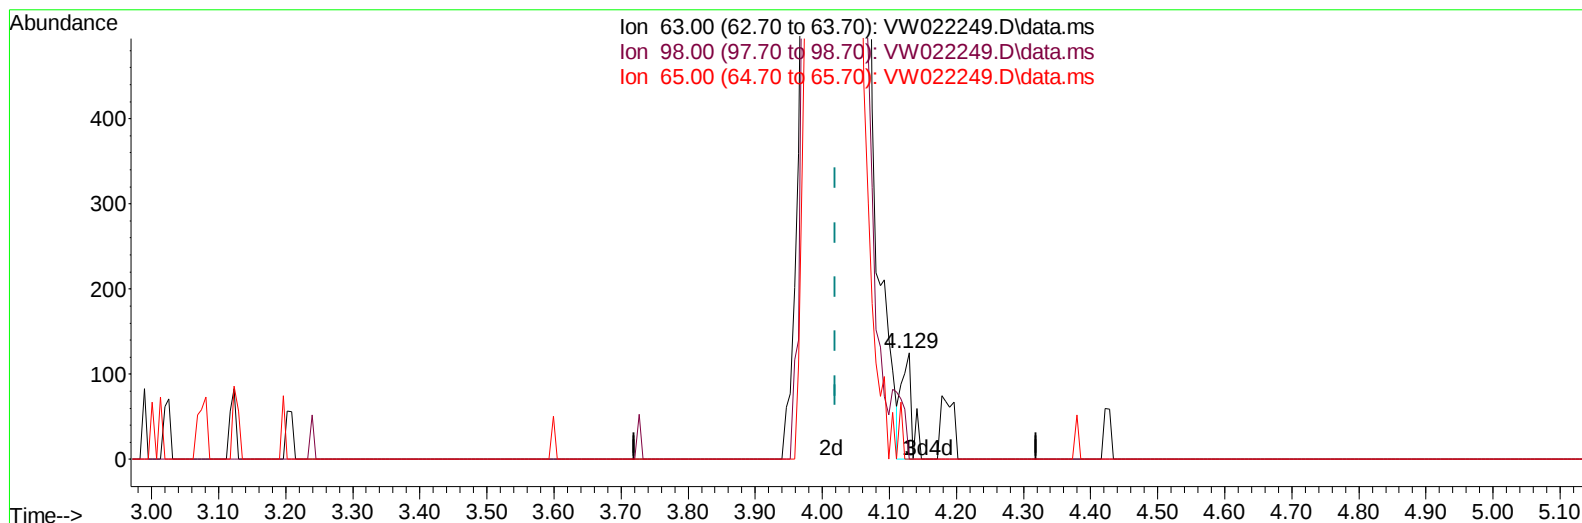

TIC: VW022249.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.129min (+ 0.110) 0.03 ug/L

response 115

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	78.60	92.17
65.00	24.30	20.87
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022249.D
Acq On : 09 Mar 2022 13:32
Operator : SY/VA
Sample : N1818-13
Misc : 6.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF7

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

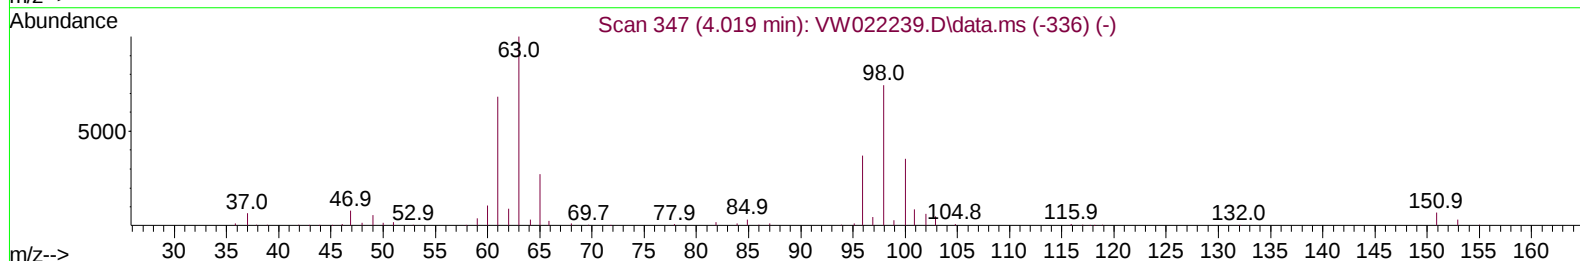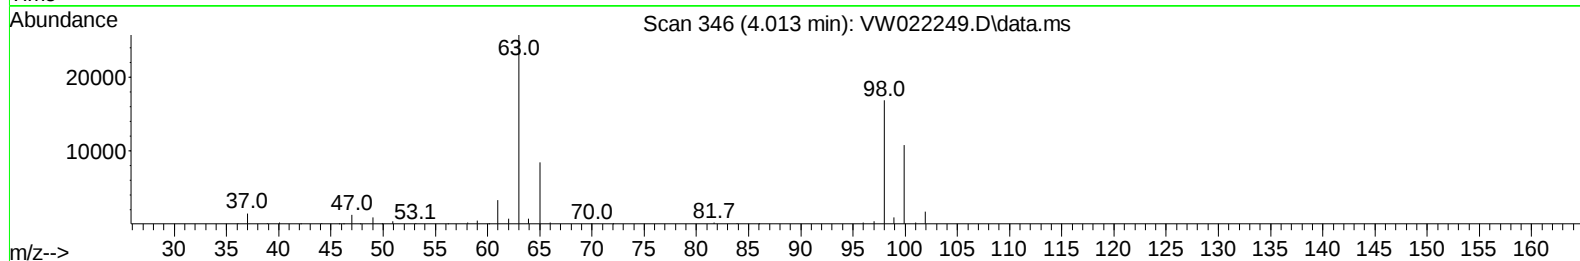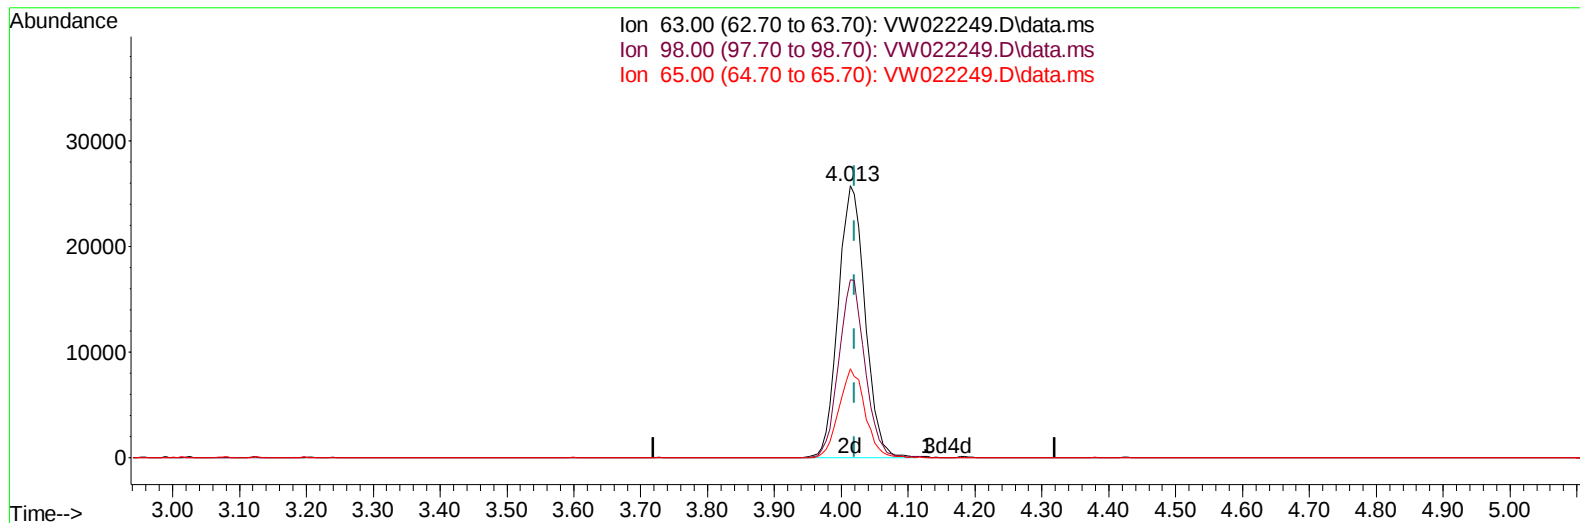

TIC: VW022249.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 18.64 ug/L m

response 71505

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	78.60	0.15#
65.00	24.30	0.03#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022249.D
Acq On : 09 Mar 2022 13:32
Operator : SY/VA
Sample : N1818-13
Misc : 6.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF7

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

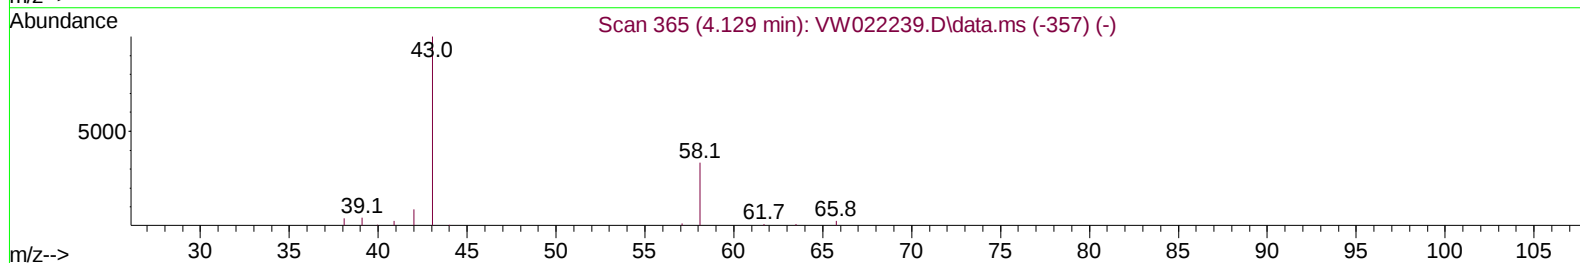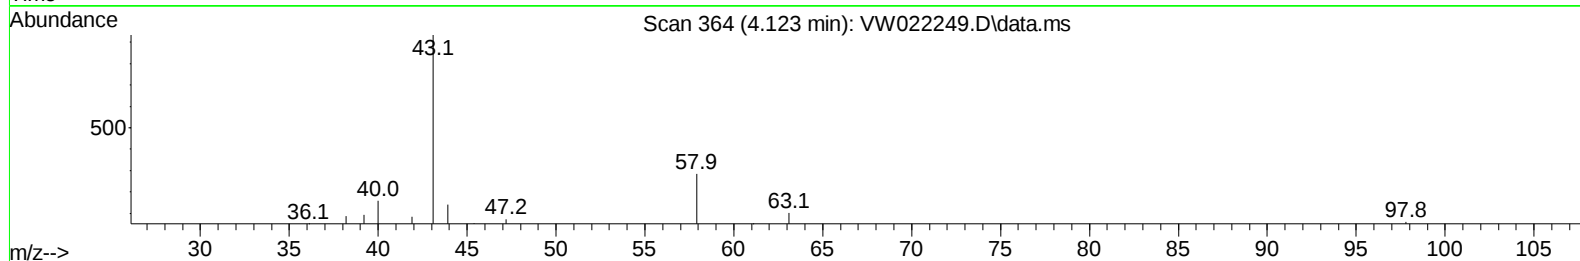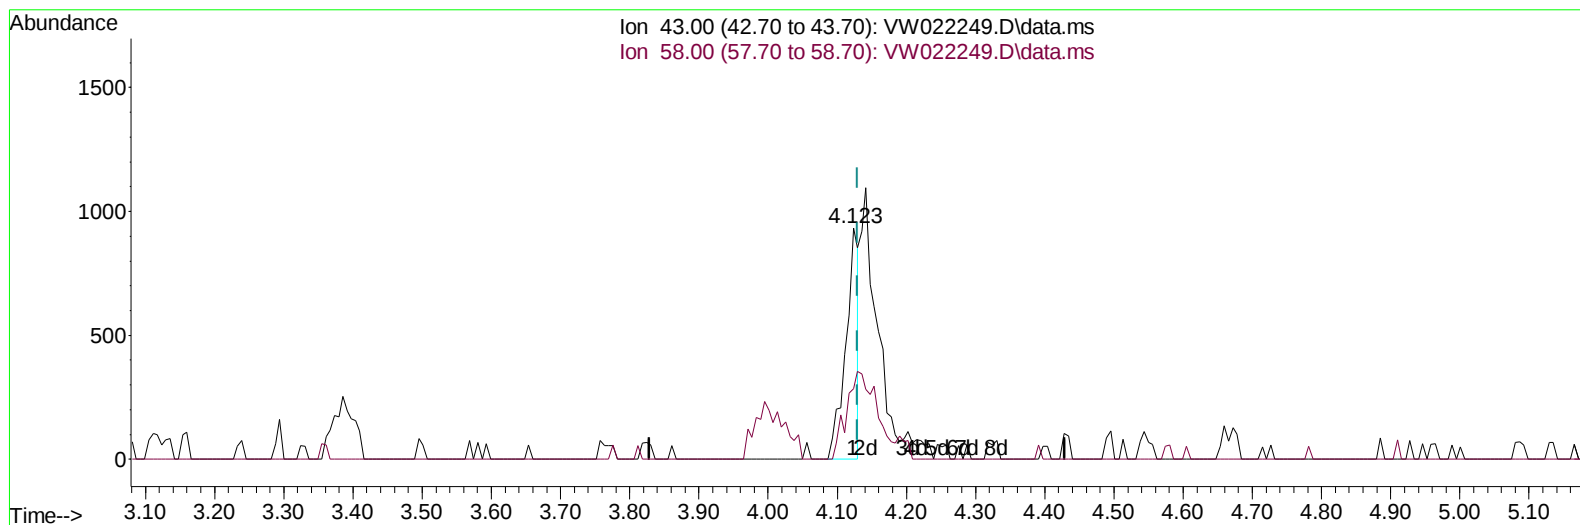

TIC: VW022249.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 3.49 ug/L

response 1202

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	65.47
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022249.D
Acq On : 09 Mar 2022 13:32
Operator : SY/VA
Sample : N1818-13
Misc : 6.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF7

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

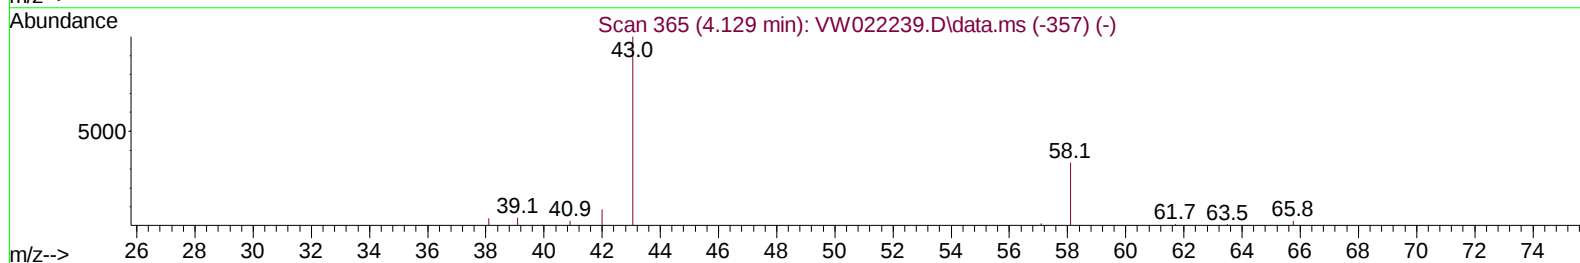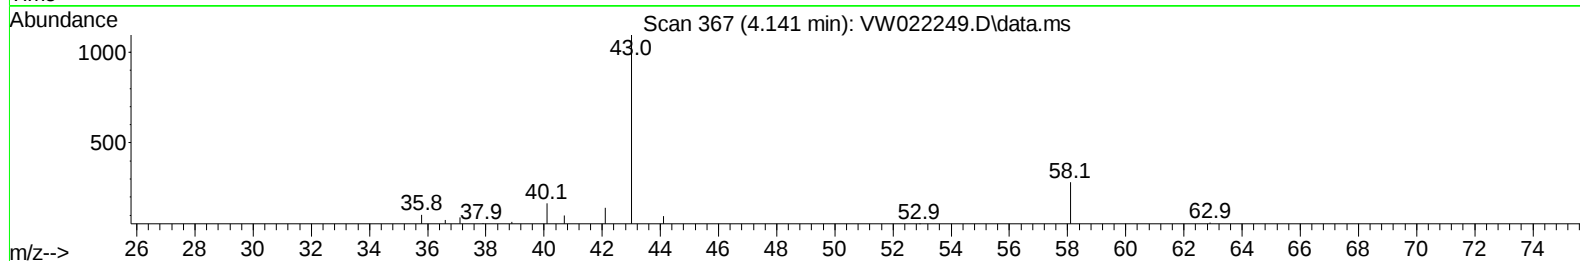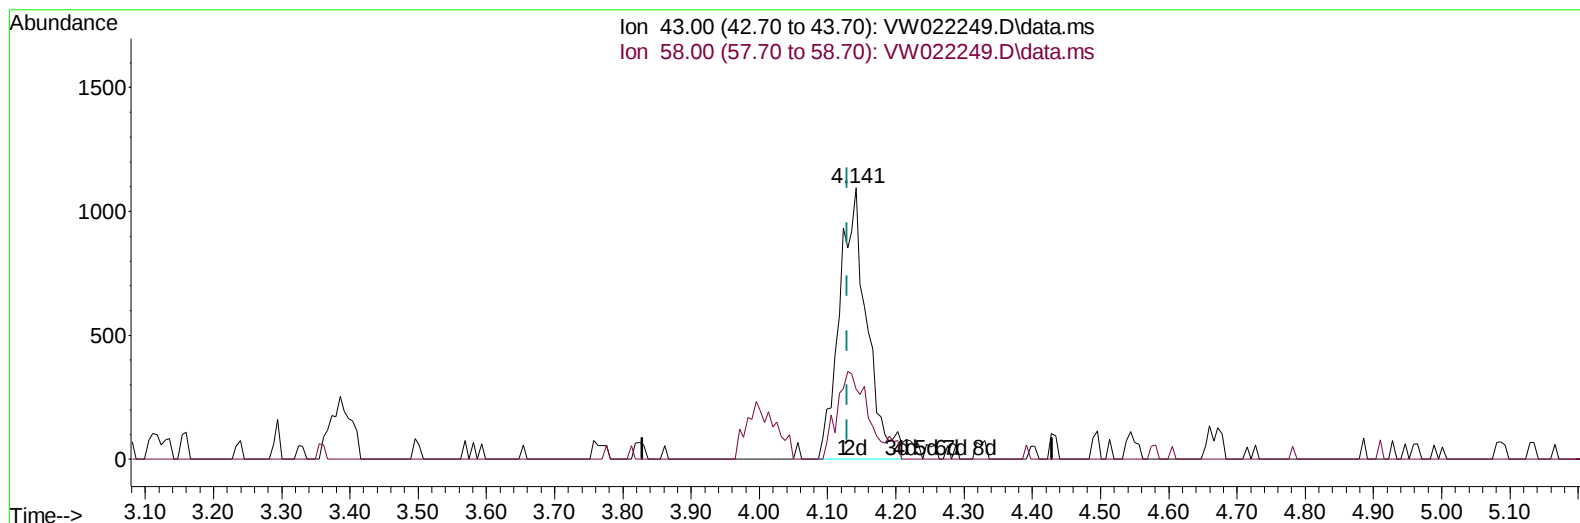

TIC: VW022249.D\data.ms

(13) Acetone (T)

4.141min (+ 0.012) 8.91 ug/L m

response 3064

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	25.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022249.D
 Acq On : 09 Mar 2022 13:32
 Operator : SY/VA
 Sample : N1818-13
 Misc : 6.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF7

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	192088	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	179173	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	84537	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	73958	29.519	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	118.080%	
7) Chloroethane-d5	2.879	69	48930	24.821	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	99.280%	
11) 1,1-Dichloroethene-d2	4.013	63	71505m	18.637	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	74.560%	
21) 2-Butanone-d5	7.080	46	20158	47.853	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	95.700%	
24) Chloroform-d	7.647	84	103151	24.068	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.280%	
26) 1,2-Dichloroethane-d4	8.305	65	54512	24.469	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.880%	
32) Benzene-d6	8.275	84	205750	24.674	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	98.680%	
36) 1,2-Dichloropropane-d6	9.275	67	56312	24.317	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	97.280%	
41) Toluene-d8	10.323	98	200217	24.151	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	96.600%	
43) trans-1,3-Dichloroprop...	10.579	79	24161	23.531	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	94.120%	
47) 2-Hexanone-d5	10.921	63	16359	42.951	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	85.900%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	46154	22.710	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	90.840%	
66) 1,2-Dichlorobenzene-d4	13.853	152	69856	25.727	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	102.920%	
Target Compounds					Qvalue	
13) Acetone	4.141	43	3064m	8.906	ug/L	
14) Carbon disulfide	4.379	76	9017	1.753	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022249.D
Acq On : 09 Mar 2022 13:32
Operator : SY/VA
Sample : N1818-13
Misc : 6.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:14:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

