




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022250.D
 Acq On : 09 Mar 2022 13:56
 Operator : SY/VA
 Sample : N1818-06
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:14:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

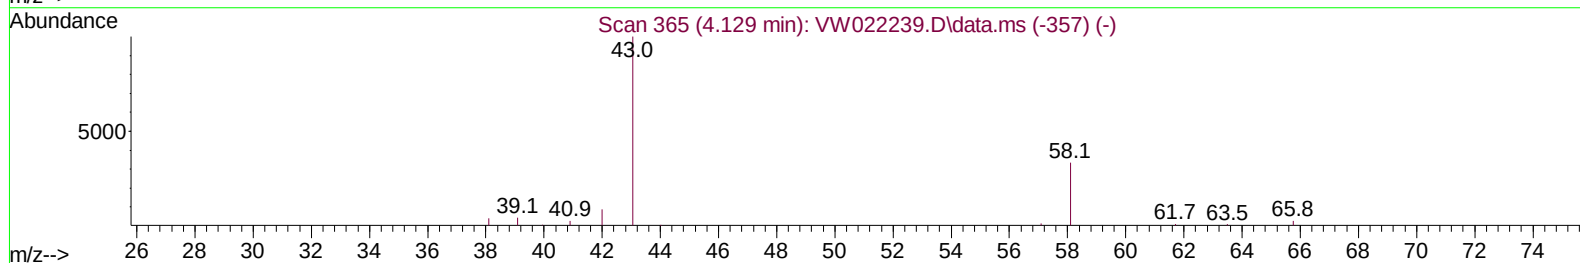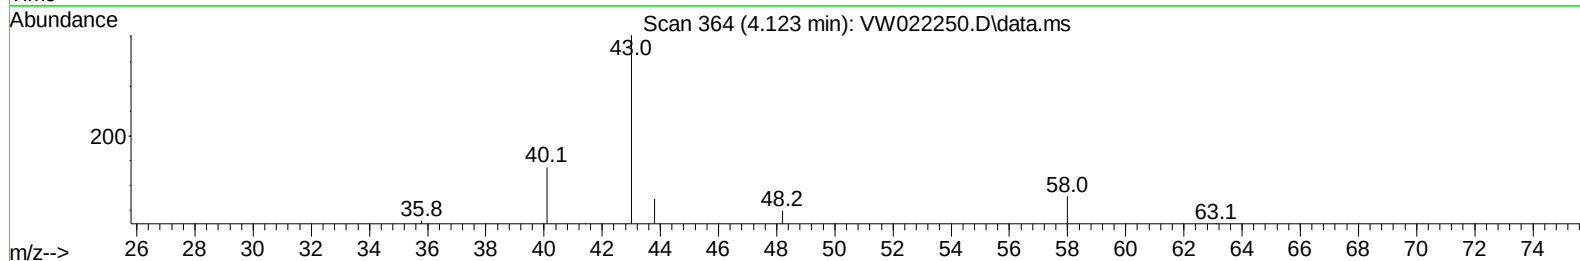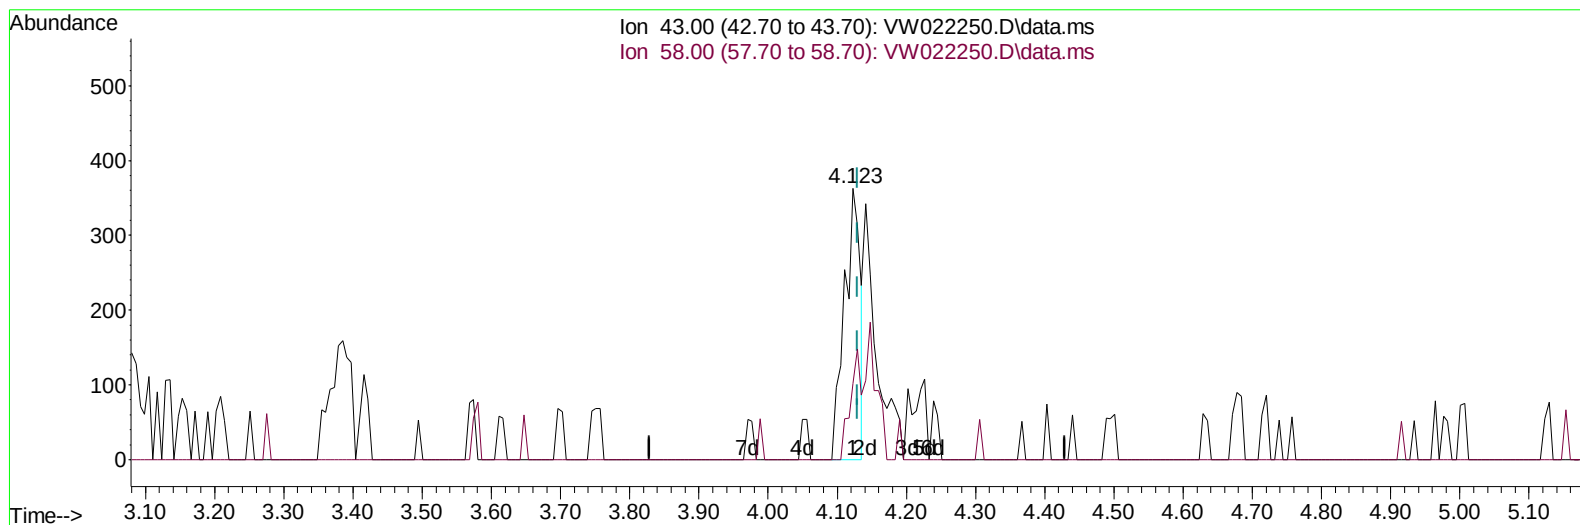

TIC: VW022250.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 2.13 ug/L

response 585

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	28.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022250.D
 Acq On : 09 Mar 2022 13:56
 Operator : SY/VA
 Sample : N1818-06
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF2

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

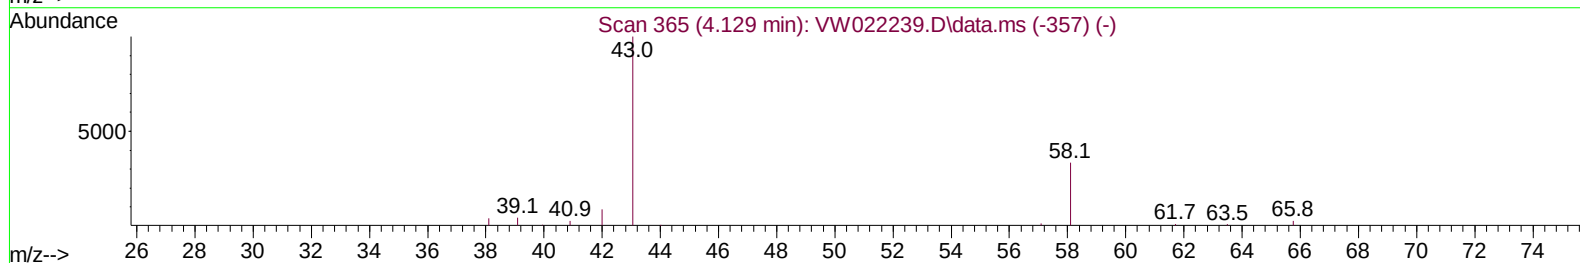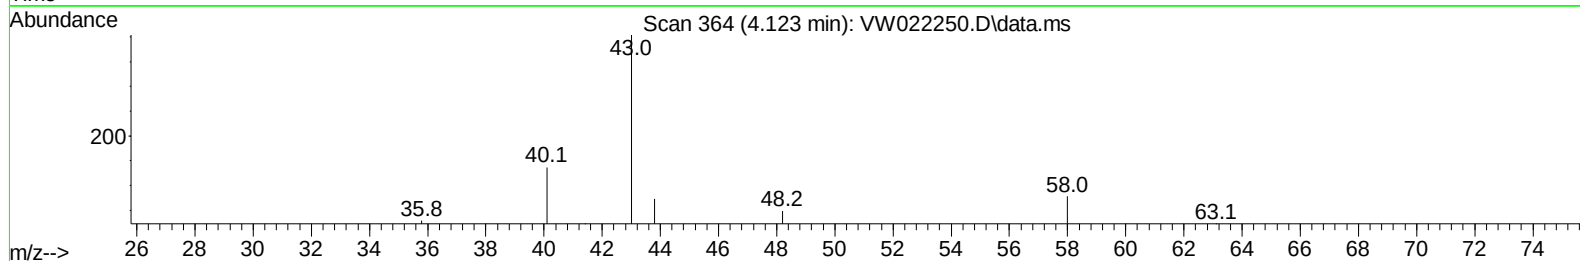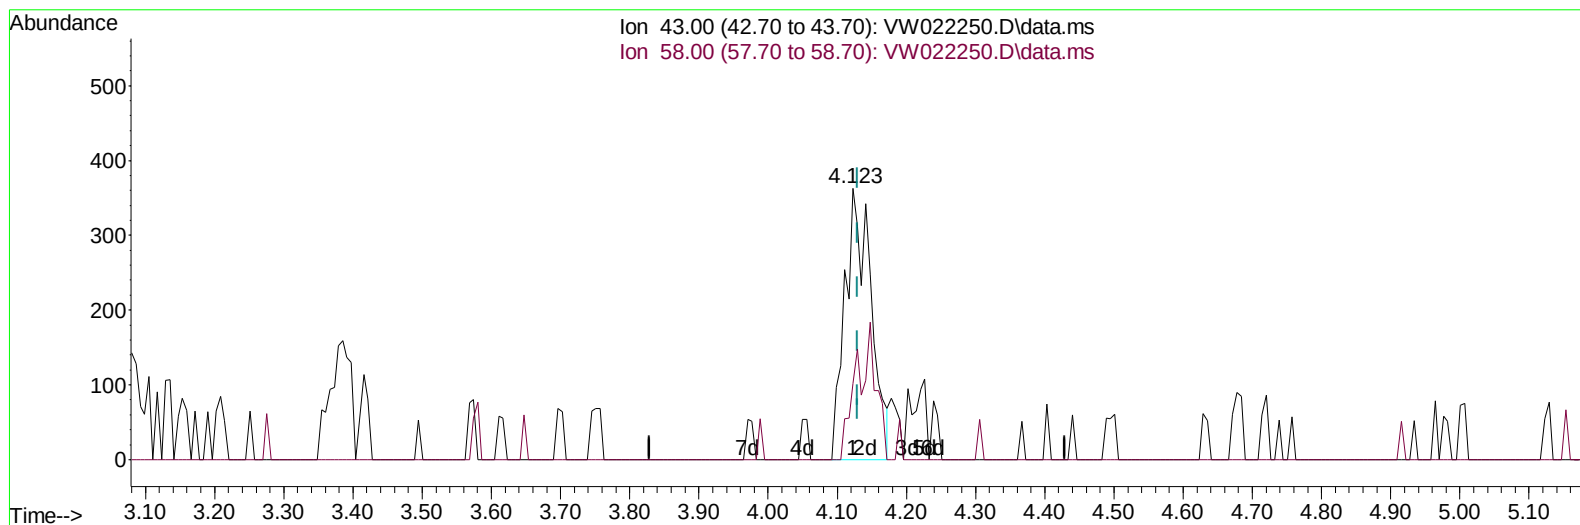

TIC: VW022250.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 3.45 ug/L m

response 950

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	17.26
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022250.D
 Acq On : 09 Mar 2022 13:56
 Operator : SY/VA
 Sample : N1818-06
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF2

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:14:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		153637	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		146420	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		69031	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		53232	26.564	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.240%	
7) Chloroethane-d5	2.879	69		33949	21.532	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.120%	
11) 1,1-Dichloroethene-d2	4.013	63		50313	16.395	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.600%	
21) 2-Butanone-d5	7.080	46		19634	58.274	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.540%	
24) Chloroform-d	7.647	84		74411	21.708	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.840%	
26) 1,2-Dichloroethane-d4	8.305	65		44369	24.901	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.600%	
32) Benzene-d6	8.275	84		149560	21.948	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.800%	
36) 1,2-Dichloropropane-d6	9.274	67		40988	21.659	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.640%	
41) Toluene-d8	10.323	98		144880	21.385	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.560%	
43) trans-1,3-Dichloroprop...	10.579	79		18526	22.079	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.320%	
47) 2-Hexanone-d5	10.927	63		15693	50.419	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.840%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		40416	24.335	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.320%	
66) 1,2-Dichlorobenzene-d4	13.853	152		52931	23.873	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.480%	
Target Compounds							Qvalue
13) Acetone	4.123	43		950m	3.452	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022250.D
Acq On : 09 Mar 2022 13:56
Operator : SY/VA
Sample : N1818-06
Misc : 6.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:14:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

