




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022252.D
 Acq On : 09 Mar 2022 14:44
 Operator : SY/VA
 Sample : N1818-12
 Misc : 4.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:15:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

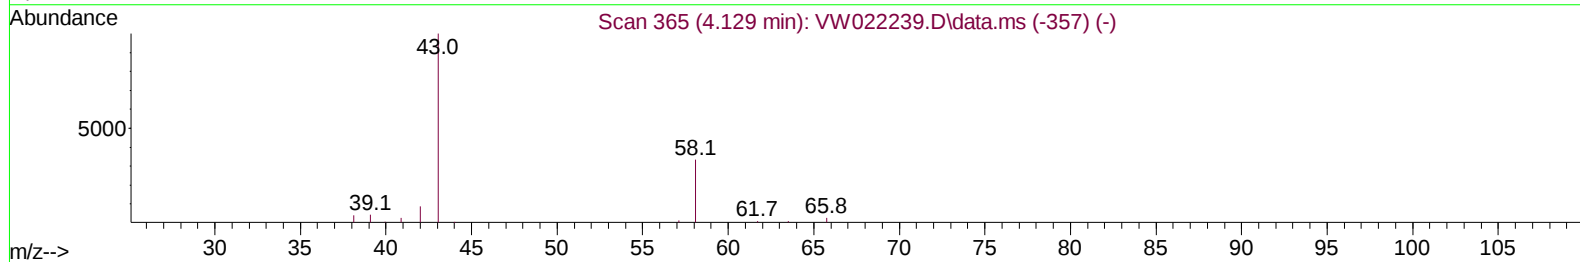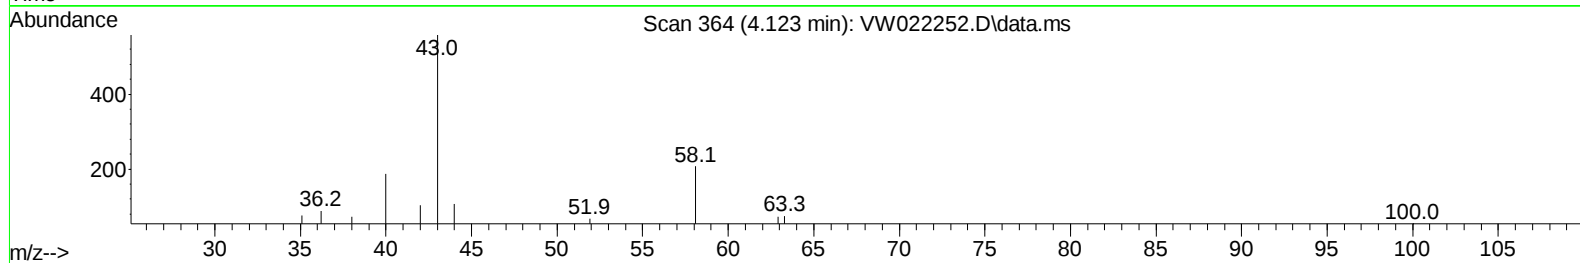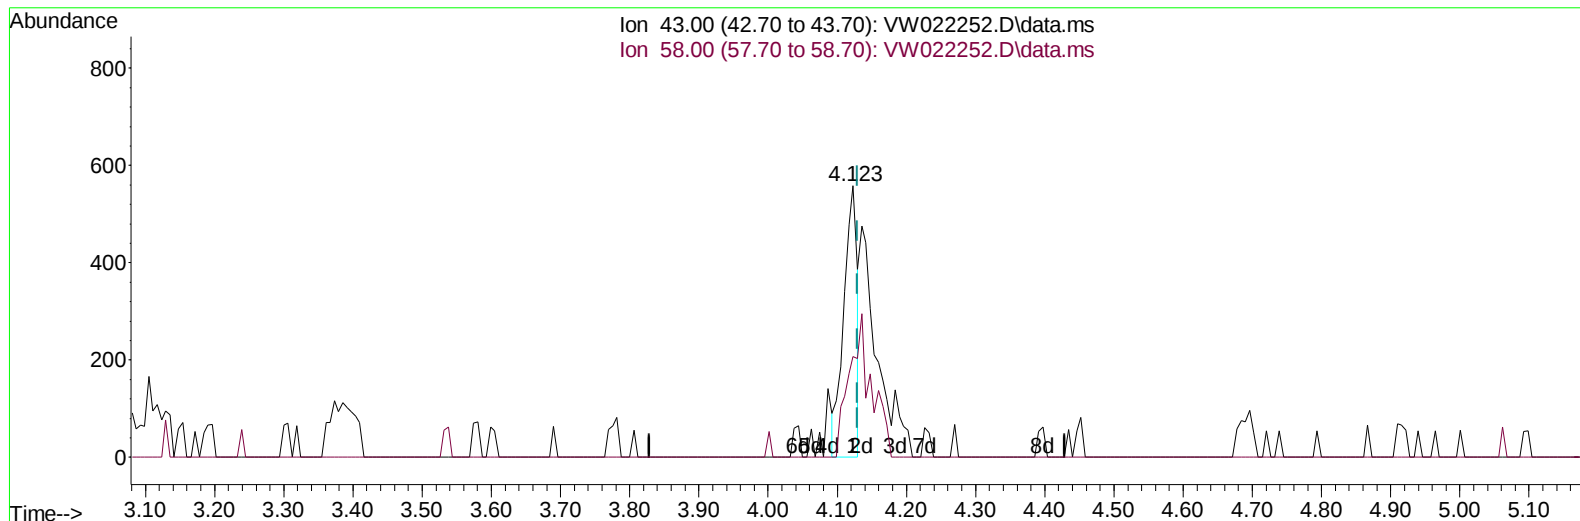

TIC: VW022252.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 2.14 ug/L

response 756

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022252.D
Acq On : 09 Mar 2022 14:44
Operator : SY/VA
Sample : N1818-12
Misc : 4.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:15:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

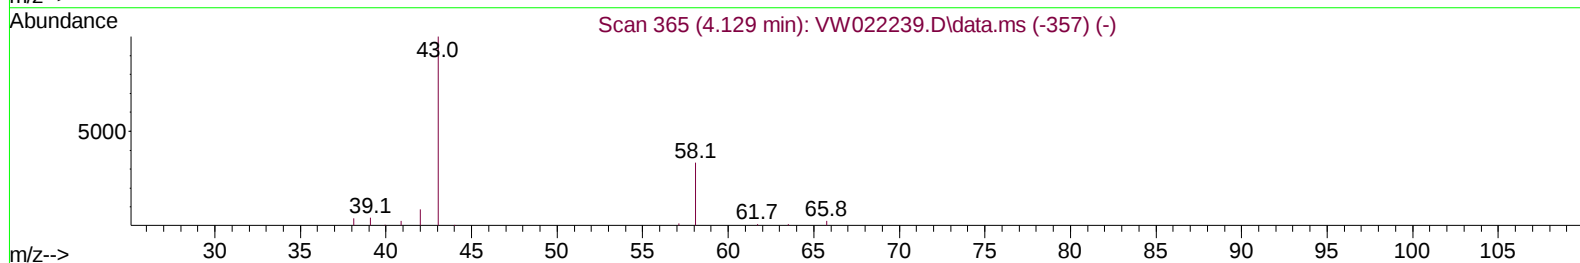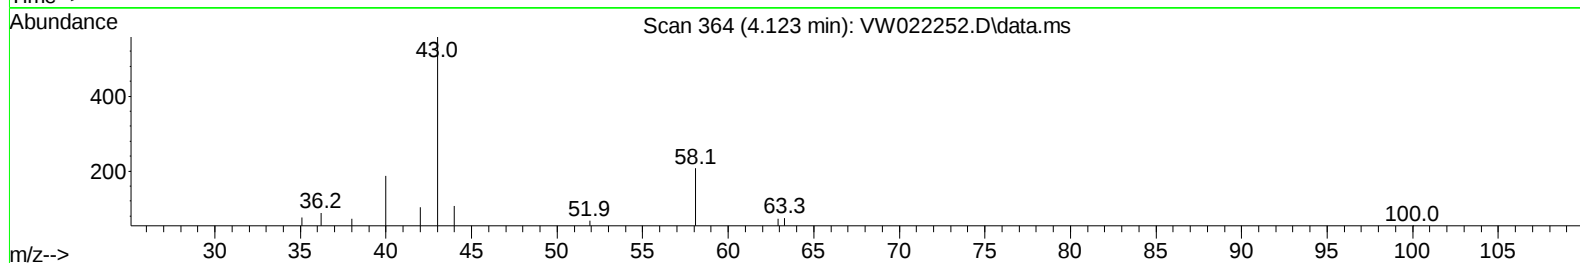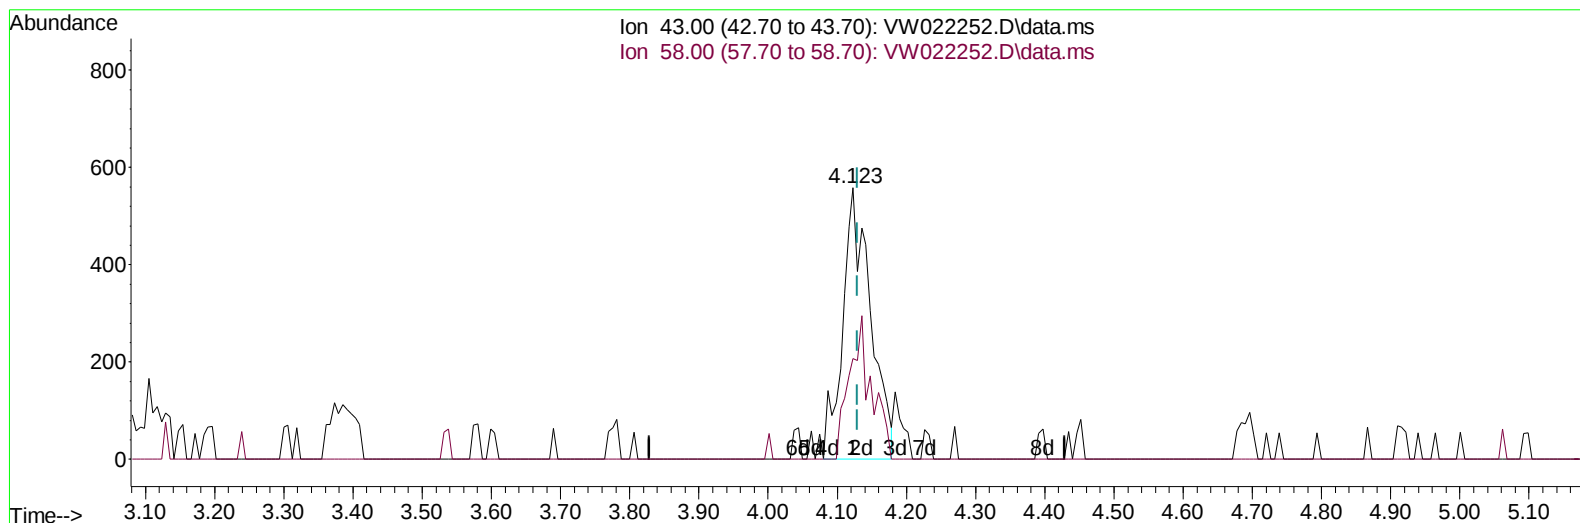

TIC: VW022252.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.42 ug/L m

response 1561

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022252.D
 Acq On : 09 Mar 2022 14:44
 Operator : SY/VA
 Sample : N1818-12
 Misc : 4.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:15:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		197244	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		178913	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		85918	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		76969	29.918	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	119.680%	
7) Chloroethane-d5	2.879	69		51472	25.428	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	101.720%	
11) 1,1-Dichloroethene-d2	4.013	63		73336	18.614	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	74.440%	
21) 2-Butanone-d5	7.074	46		19863	45.920	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	91.840%	
24) Chloroform-d	7.647	84		105225	23.910	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	95.640%	
26) 1,2-Dichloroethane-d4	8.305	65		56278	24.602	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	98.400%	
32) Benzene-d6	8.275	84		216968	26.057	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	104.240%	
36) 1,2-Dichloropropane-d6	9.274	67		58474	25.287	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	101.160%	
41) Toluene-d8	10.323	98		207516	25.068	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	100.280%	
43) trans-1,3-Dichloroprop...	10.579	79		23755	23.169	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	92.680%	
47) 2-Hexanone-d5	10.921	63		16160	42.490	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	84.980%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		45670	22.504	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	90.000%	
66) 1,2-Dichlorobenzene-d4	13.853	152		69772	25.283	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	101.120%	
Target Compounds							
13) Acetone	4.123	43		1561m	4.418	ug/L	
17) trans-1,2-Dichloroethene	5.422	96		9111	4.071	ug/L	90
20) cis-1,2-Dichloroethene	7.171	96		6112	2.521	ug/L	95
34) Trichloroethene	9.092	95		13511	5.455	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022252.D
Acq On : 09 Mar 2022 14:44
Operator : SY/VA
Sample : N1818-12
Misc : 4.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:15:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

