




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022257.D
Acq On : 09 Mar 2022 16:45
Operator : SY/VA
Sample : N1818-19
Misc : 6.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG7

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:16:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

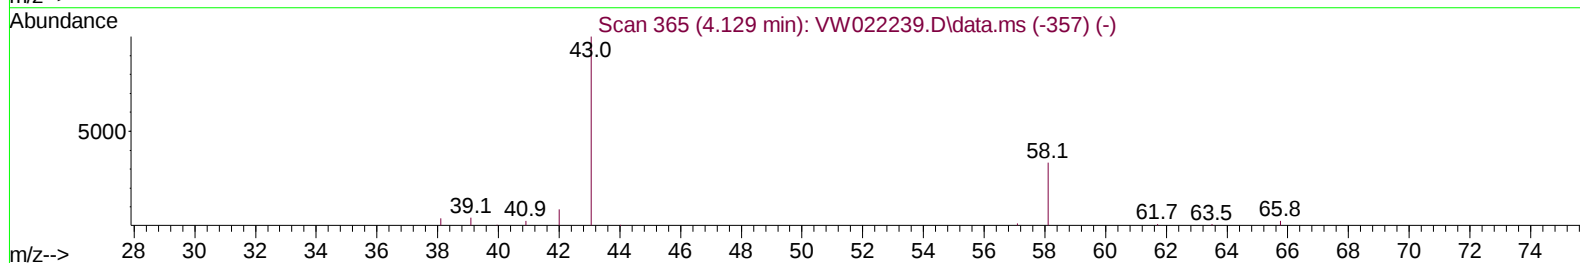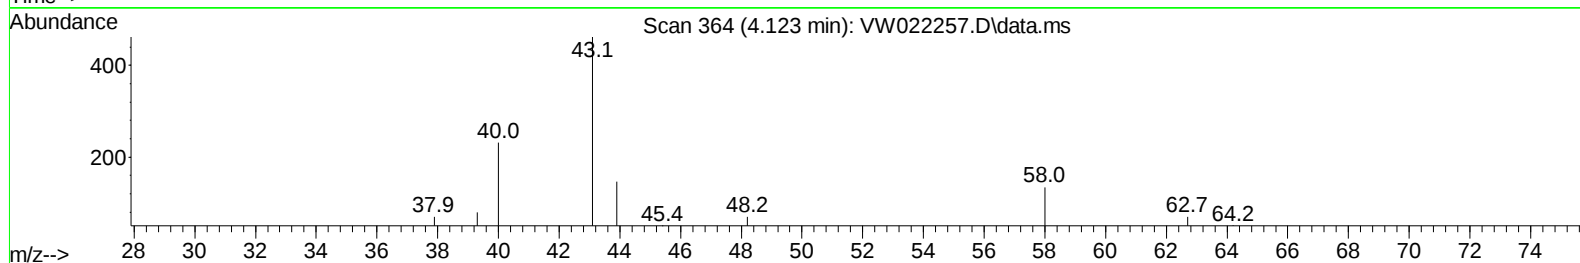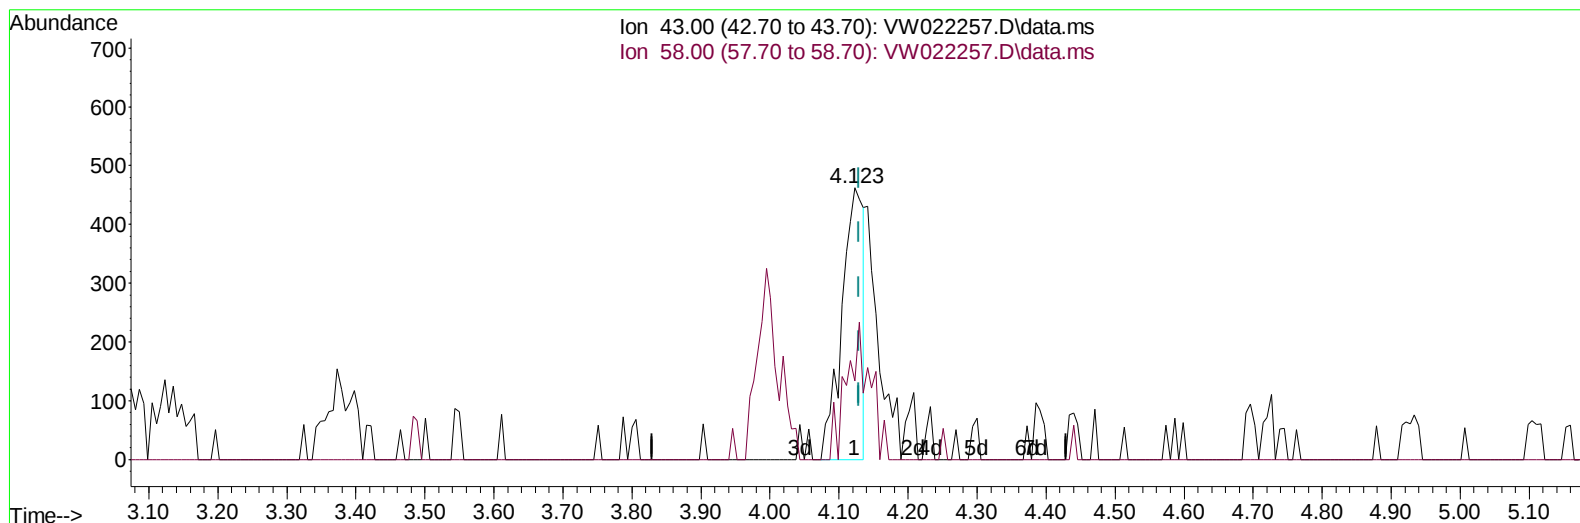

TIC: VW022257.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 2.85 ug/L

response 1007

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	12.61
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022257.D
Acq On : 09 Mar 2022 16:45
Operator : SY/VA
Sample : N1818-19
Misc : 6.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG7

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:16:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

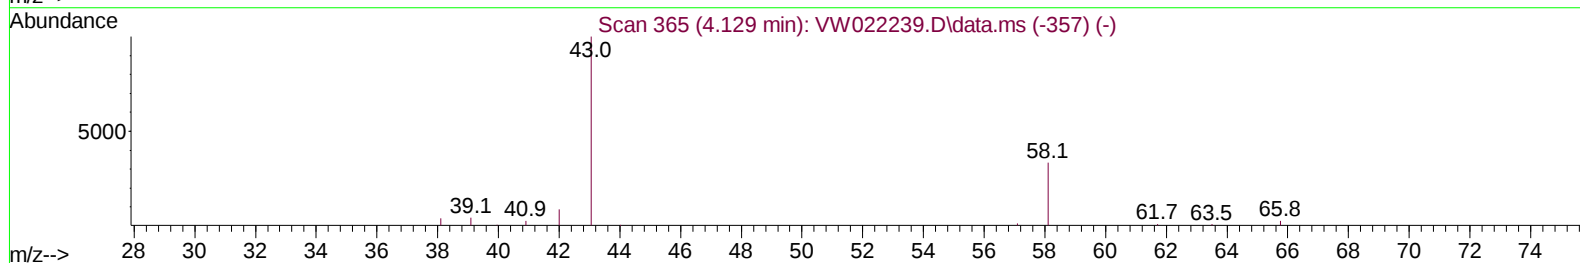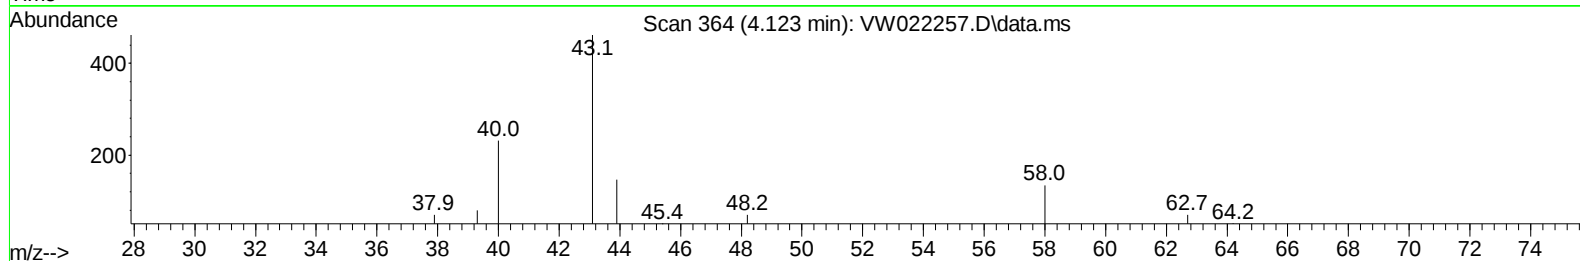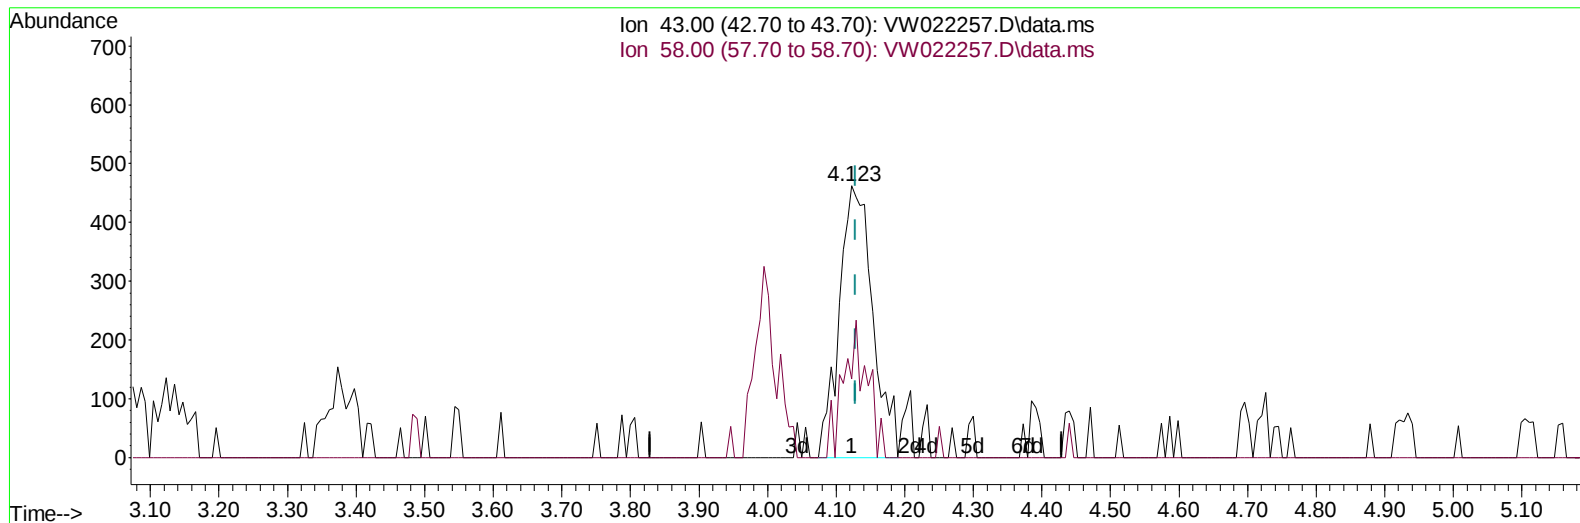

TIC: VW022257.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.45 ug/L m

response 1570

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	8.09
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022257.D
 Acq On : 09 Mar 2022 16:45
 Operator : SY/VA
 Sample : N1818-19
 Misc : 6.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:16:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		196968	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		179010	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		86364	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		67750	26.371	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.480%	
7) Chloroethane-d5	2.879	69		47235	23.368	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.480%	
11) 1,1-Dichloroethene-d2	4.013	63		67982	17.280	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.120%	
21) 2-Butanone-d5	7.080	46		25181	58.296	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.600%	
24) Chloroform-d	7.647	84		100206	22.802	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.200%	
26) 1,2-Dichloroethane-d4	8.305	65		54978	24.067	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.280%	
32) Benzene-d6	8.275	84		202414	24.296	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.200%	
36) 1,2-Dichloropropane-d6	9.274	67		55220	23.867	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.480%	
41) Toluene-d8	10.323	98		192547	23.247	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.000%	
43) trans-1,3-Dichloroprop...	10.579	79		23540	22.947	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.800%	
47) 2-Hexanone-d5	10.920	63		19972	52.485	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.960%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		51141	25.187	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.760%	
66) 1,2-Dichlorobenzene-d4	13.853	152		69604	25.092	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.360%	
Target Compounds							
13) Acetone	4.123	43		1570m	4.450	ug/L	
46) Tetrachloroethene	10.859	164		1170	0.539	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022257.D
Acq On : 09 Mar 2022 16:45
Operator : SY/VA
Sample : N1818-19
Misc : 6.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:16:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

