




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022261.D
 Acq On : 09 Mar 2022 18:21
 Operator : SY/VA
 Sample : N1838-02
 Misc : 5.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0QA0

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:16:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

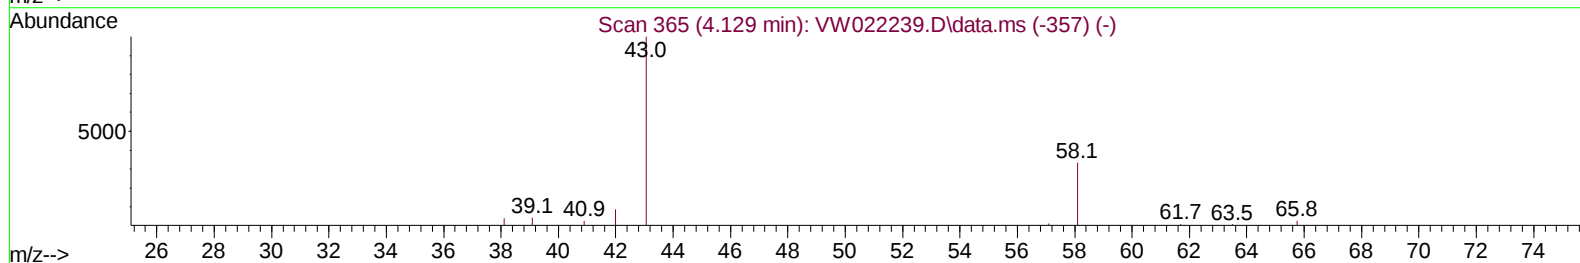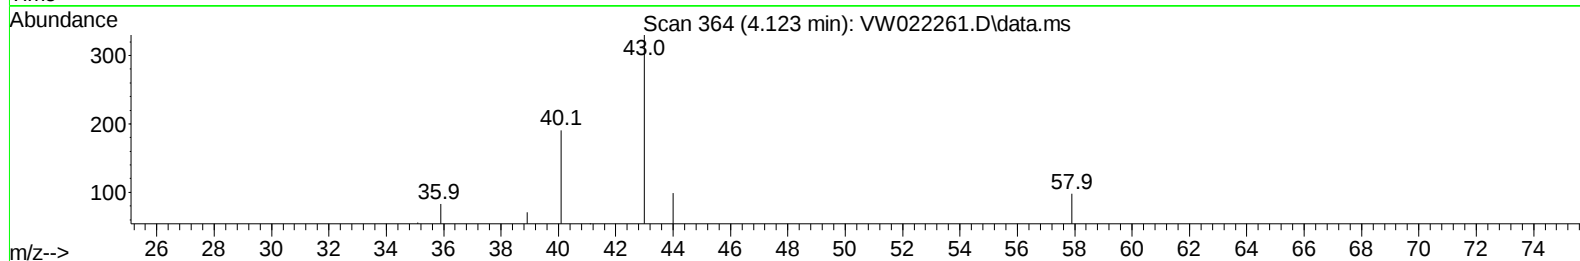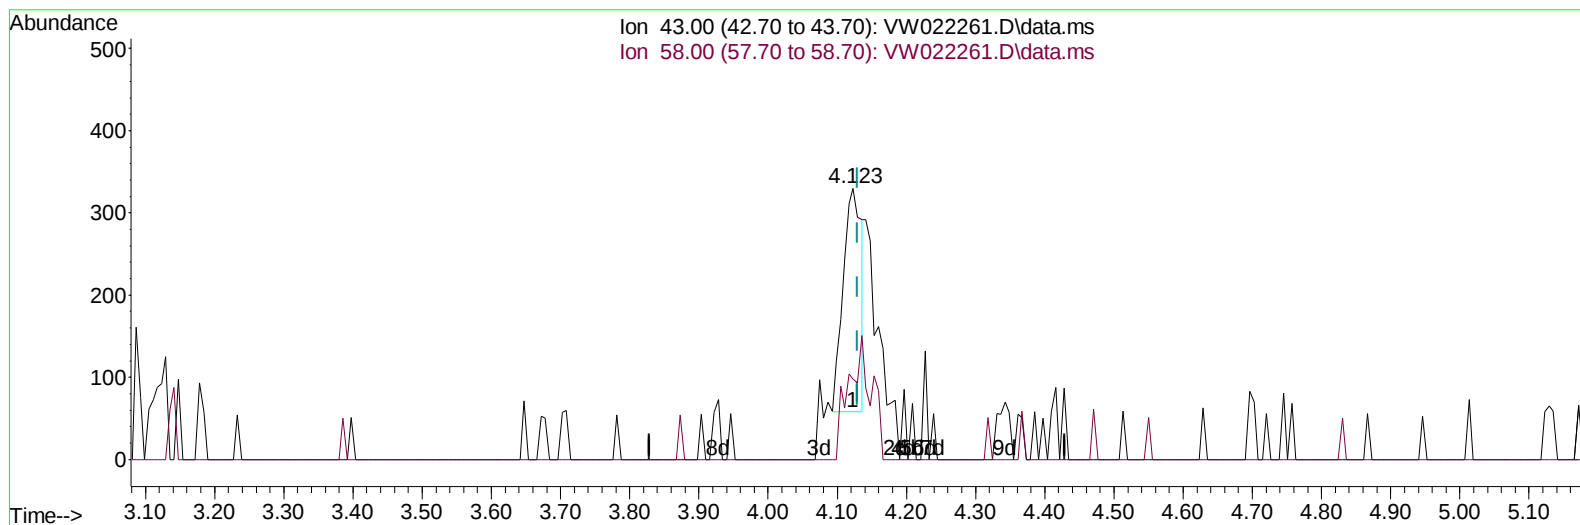

TIC: VW022261.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 1.94 ug/L

response 496

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	33.06
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022261.D
 Acq On : 09 Mar 2022 18:21
 Operator : SY/VA
 Sample : N1838-02
 Misc : 5.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0QA0

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:16:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

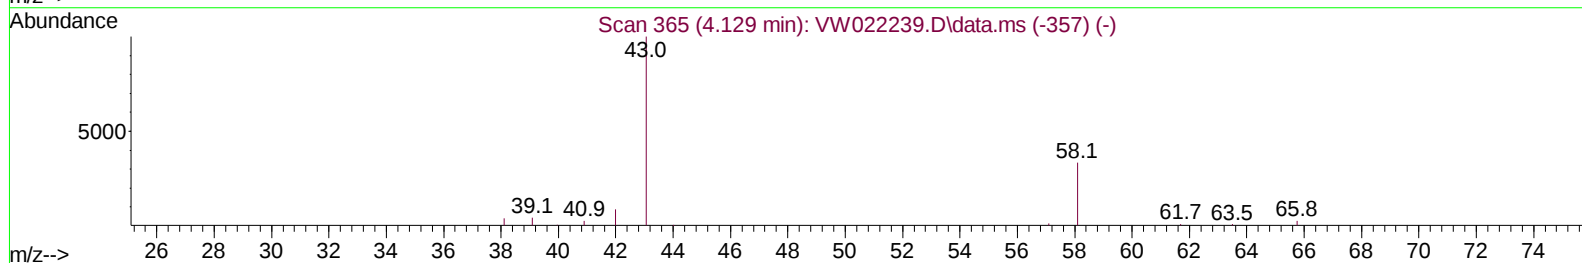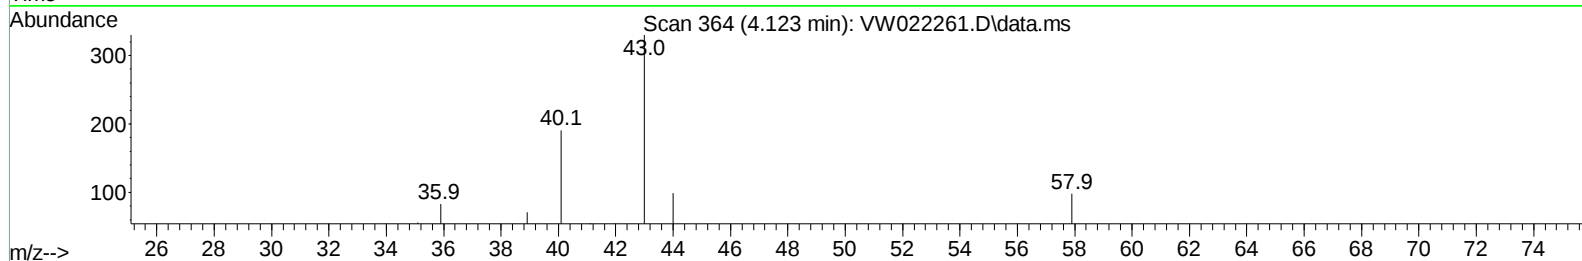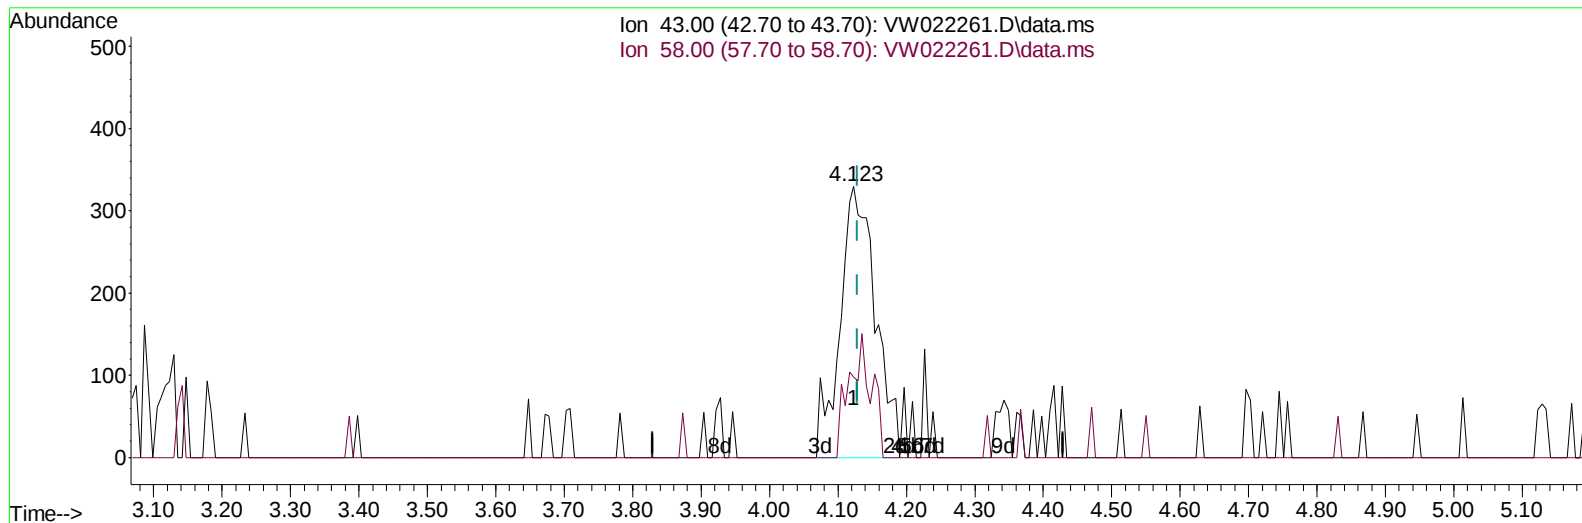

TIC: VW022261.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.64 ug/L m

response 1188

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	13.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022261.D
 Acq On : 09 Mar 2022 18:21
 Operator : SY/VA
 Sample : N1838-02
 Misc : 5.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0QA0

Manual IntegrationsAPPROVED

Quant Time: Mar 10 04:16:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	143094	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	143476	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	67986	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	49868	26.719	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	106.880%	
7) Chloroethane-d5	2.879	69	33228	22.627	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	90.520%	
11) 1,1-Dichloroethene-d2	4.019	63	50575	17.695	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	70.800%	
21) 2-Butanone-d5	7.074	46	22224	70.821	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	141.640%#	
24) Chloroform-d	7.647	84	78949	24.729	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.920%	
26) 1,2-Dichloroethane-d4	8.305	65	47392	28.557	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	114.240%	
32) Benzene-d6	8.275	84	154787	23.181	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.720%	
36) 1,2-Dichloropropane-d6	9.275	67	45307	24.433	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	97.720%	
41) Toluene-d8	10.323	98	150062	22.605	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	90.400%	
43) trans-1,3-Dichloroprop...	10.579	79	20278	24.663	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	98.640%	
47) 2-Hexanone-d5	10.921	63	17523	57.454	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	114.900%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	45217	27.784	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	111.120%	
66) 1,2-Dichlorobenzene-d4	13.853	152	55416	25.378	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	101.520%	
Target Compounds						
13) Acetone	4.123	43	1188m	4.635	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022261.D
Acq On : 09 Mar 2022 18:21
Operator : SY/VA
Sample : N1838-02
Misc : 5.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0QA0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:16:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

