

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022245.D
 Acq On : 09 Mar 2022 11:56
 Operator : SY/VA
 Sample : N1816-18
 Misc : 5.87g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSE3

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/10/2022
 Supervised By : Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:13:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	189542	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	180304	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	85704	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	73633	29.784	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 119.120%			
7) Chloroethane-d5	2.879	69	46268	23.786	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 95.160%			
11) 1,1-Dichloroethene-d2	4.013	63	70417	18.600	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 74.400%			
21) 2-Butanone-d5	7.080	46	19546	47.023	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 94.040%			
24) Chloroform-d	7.647	84	100867	23.852	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 95.400%			
26) 1,2-Dichloroethane-d4	8.305	65	53350	24.269	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 97.080%			
32) Benzene-d6	8.275	84	207256	24.699	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 98.800%			
36) 1,2-Dichloropropane-d6	9.274	67	55992	24.027	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 96.120%			
41) Toluene-d8	10.323	98	204823	24.552	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 98.200%			
43) trans-1,3-Dichloroprop...	10.579	79	24649	23.856	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 95.440%			
47) 2-Hexanone-d5	10.921	63	15558	40.592	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 81.180%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	45487	22.241	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 88.960%			
66) 1,2-Dichlorobenzene-d4	13.853	152	70553	25.630	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 102.520%			
Target Compounds					Qvalue	
13) Acetone	4.129	43	3198m	9.420	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022245.D
Acq On : 09 Mar 2022 11:56
Operator : SY/VA
Sample : N1816-18
Misc : 5.87g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBSE3

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 03/10/2022
Supervised By : Mahesh Dadoda 03/14/2022


Quant Time: Mar 10 04:13:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

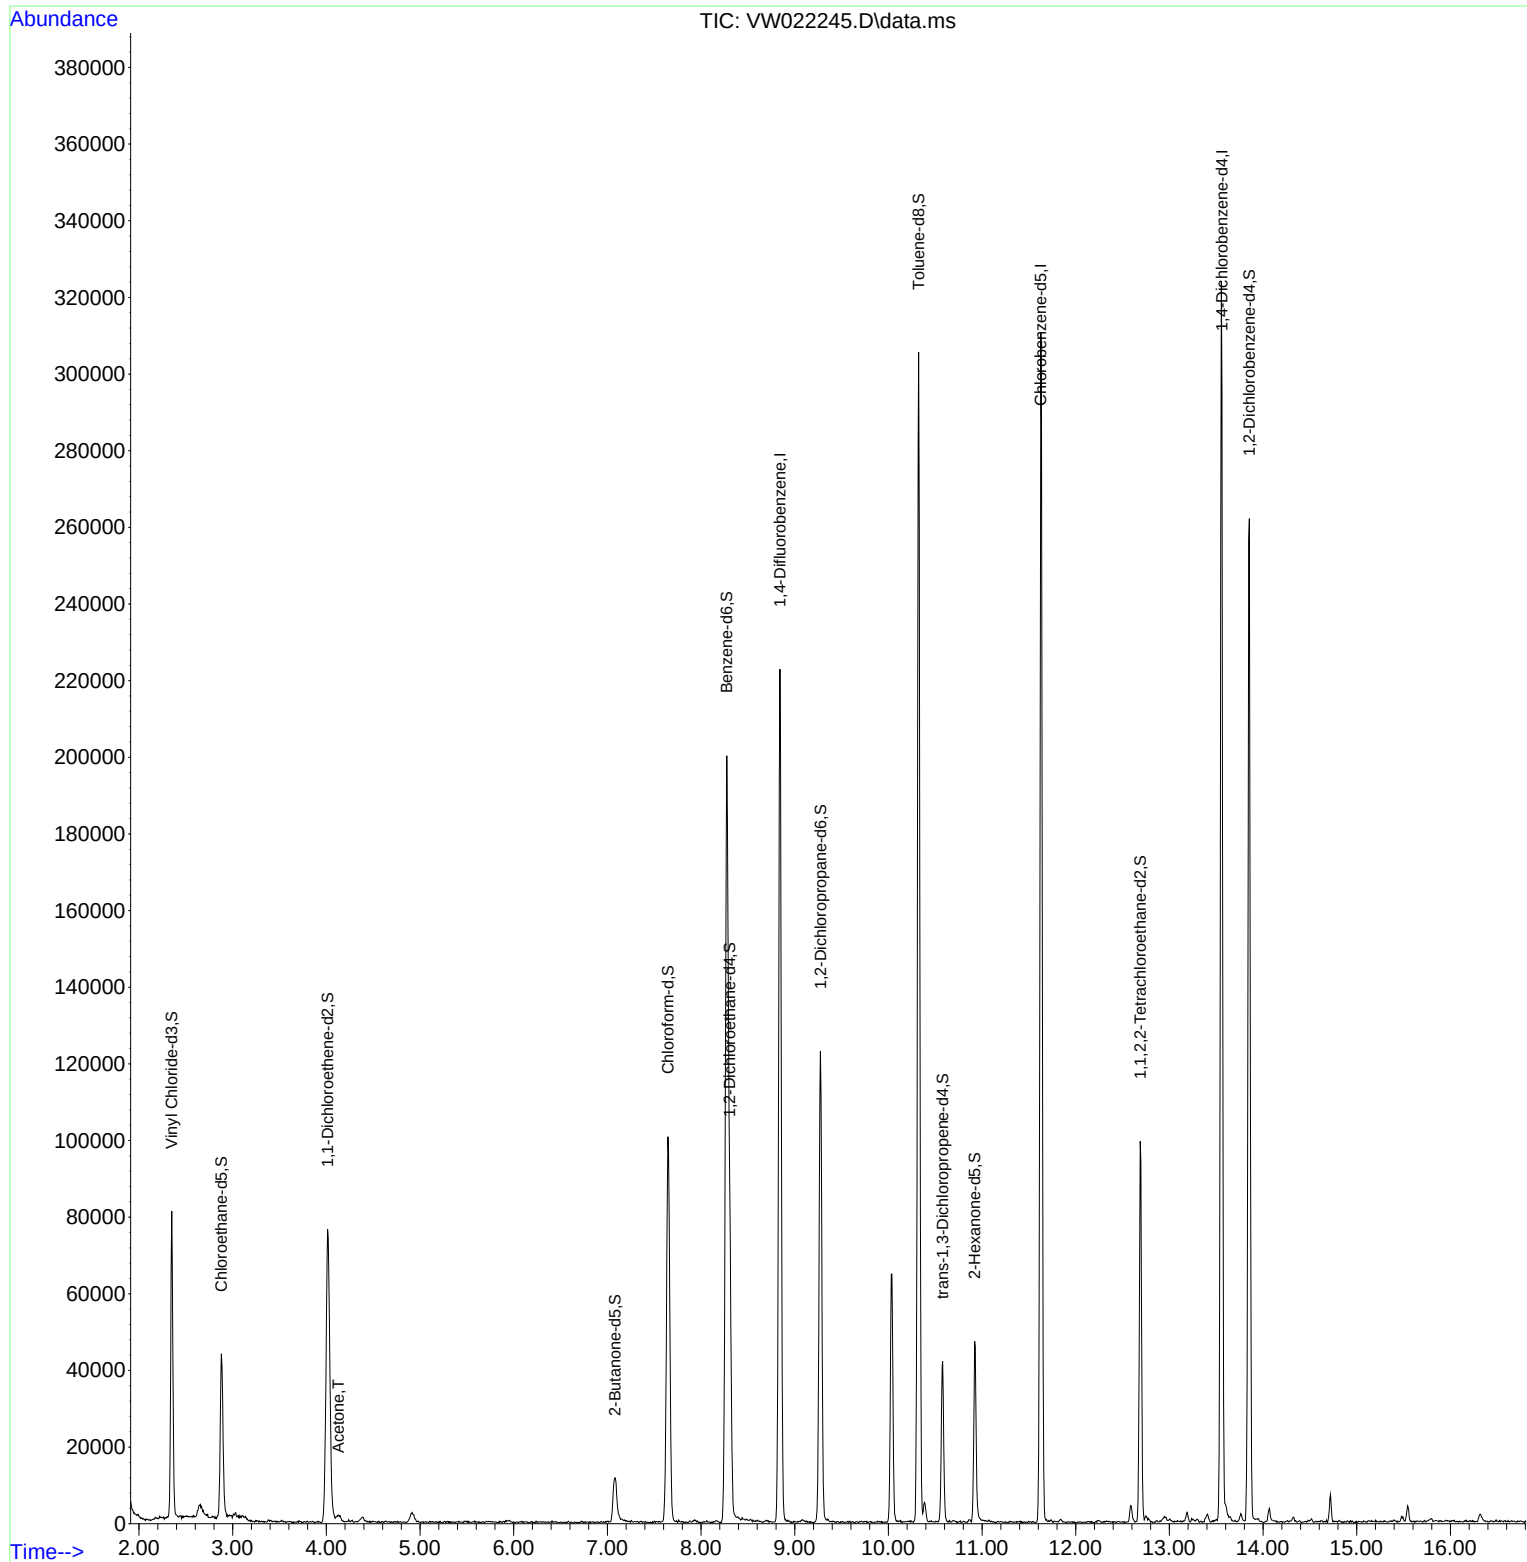

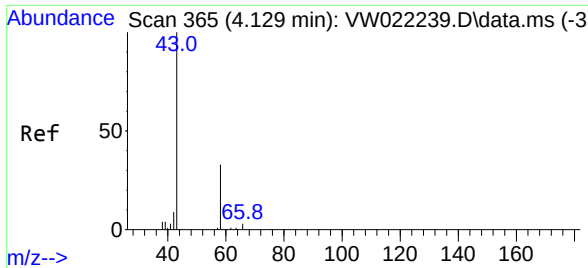

#13
Acetone
Concen: 9.420 ug/L m
RT: 4.129 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW022245.D
Acq: 09 Mar 2022 11:56

Instrument :
MSVOA_W
ClientSampleId :
DBSE3

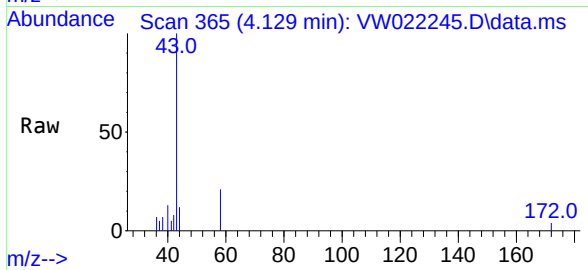

Tgt Ion: 43 Resp: 3198
Ion Ratio Lower Upper
43 100
58 30.0 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

