

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022247.D
 Acq On : 09 Mar 2022 12:44
 Operator : SY/VA
 Sample : N1818-18
 Misc : 5.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:14:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	192363	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	181373	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	89690	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	77630	30.941	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	123.760%
7) Chloroethane-d5	2.879	69	49388	25.018	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.080%
11) 1,1-Dichloroethene-d2	4.013	63	74560	19.405	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.640%
21) 2-Butanone-d5	7.073	46	19903	47.180	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.360%
24) Chloroform-d	7.646	84	110665	25.785	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.120%
26) 1,2-Dichloroethane-d4	8.305	65	57793	25.905	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.600%
32) Benzene-d6	8.274	84	221080	26.191	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.760%
36) 1,2-Dichloropropane-d6	9.268	67	59479	25.373	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.480%
41) Toluene-d8	10.323	98	216721	25.825	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.280%
43) trans-1,3-Dichloroprop...	10.579	79	24898	23.955	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.800%
47) 2-Hexanone-d5	10.920	63	17667	45.823	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.640%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	48658	23.652	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	73930	25.663	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.640%
Target Compounds					Qvalue	
13) Acetone	4.129	43	1534m	4.452	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022247.D
Acq On : 09 Mar 2022 12:44
Operator : SY/VA
Sample : N1818-18
Misc : 5.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBSG6

Quant Time: Mar 10 04:14:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

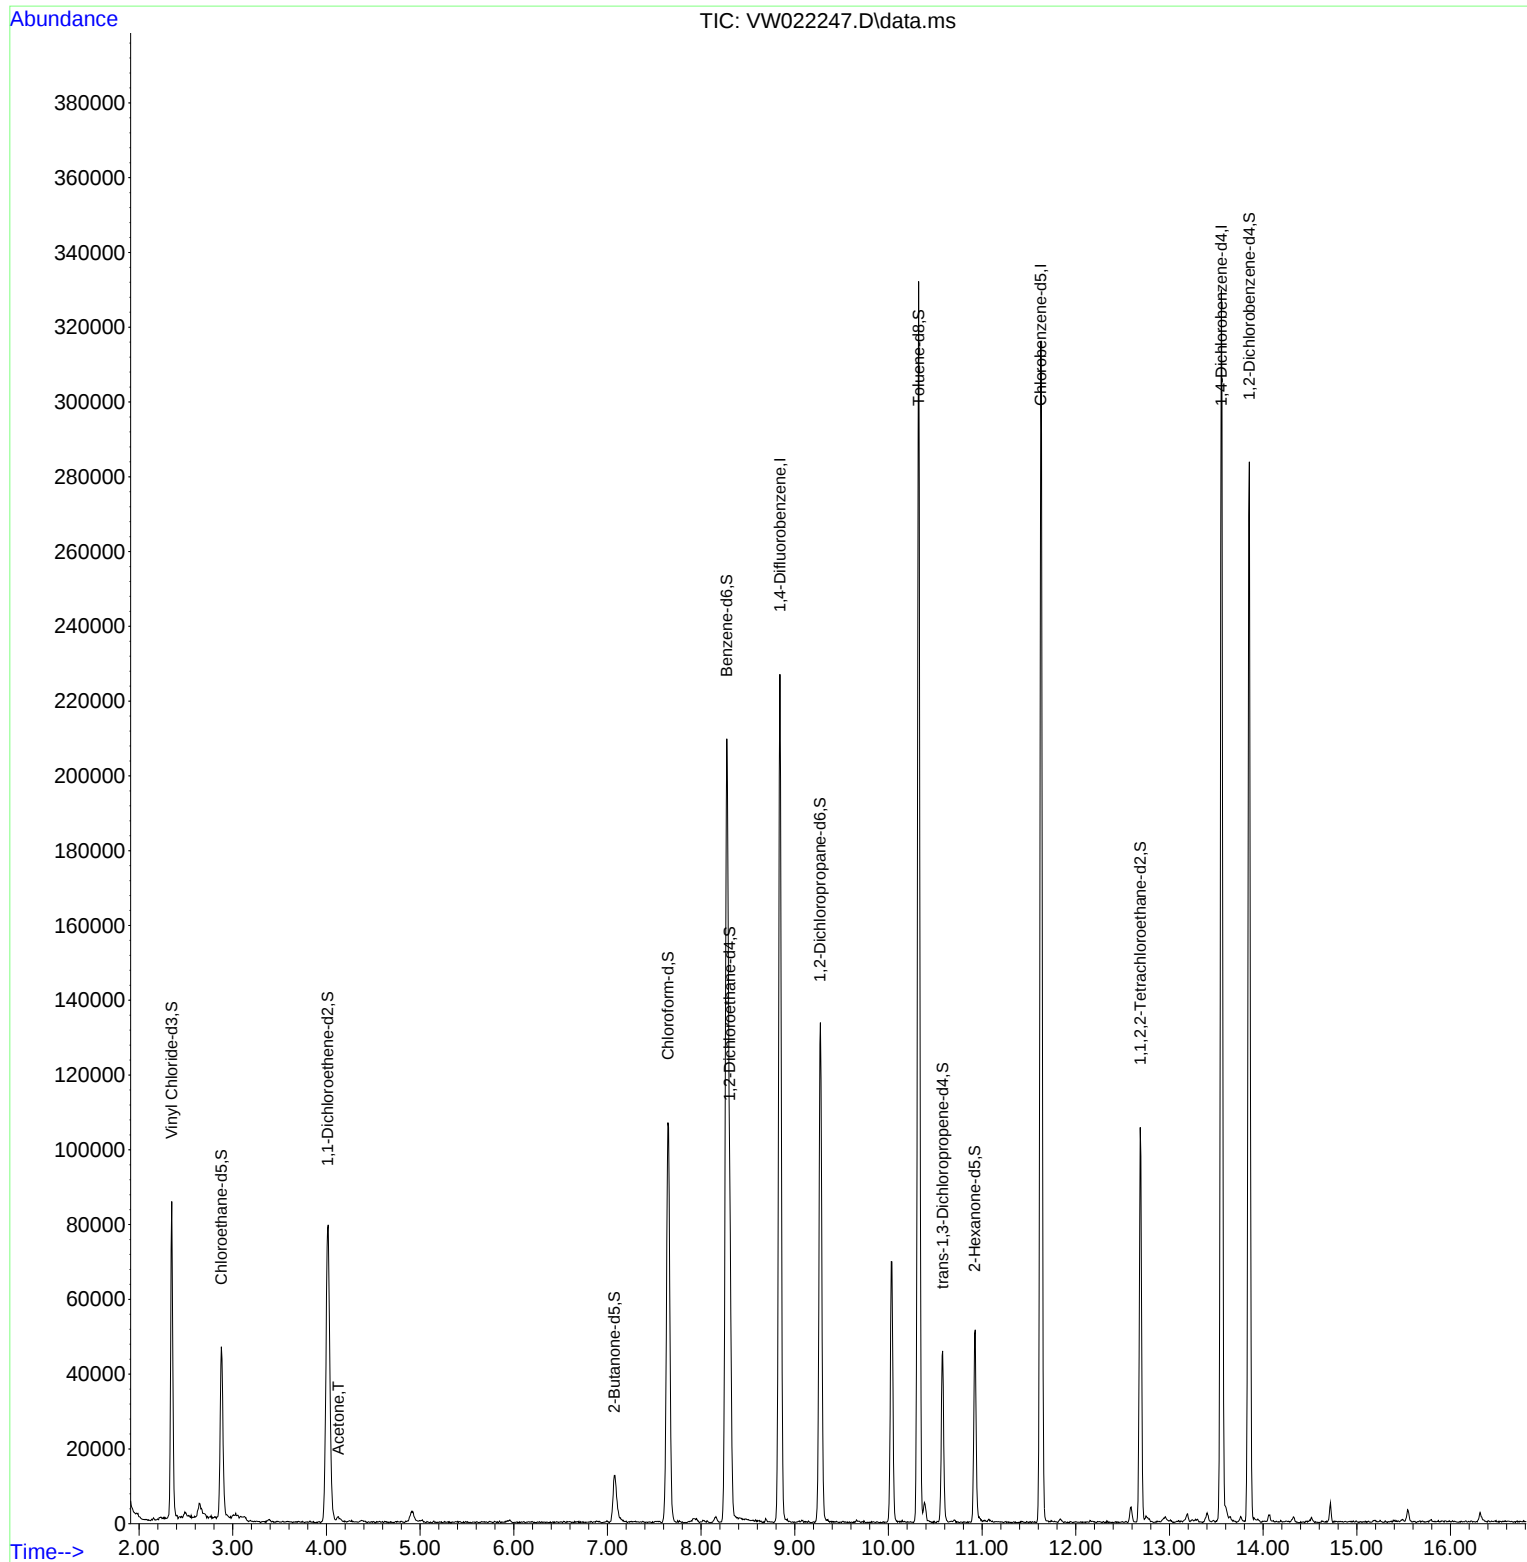

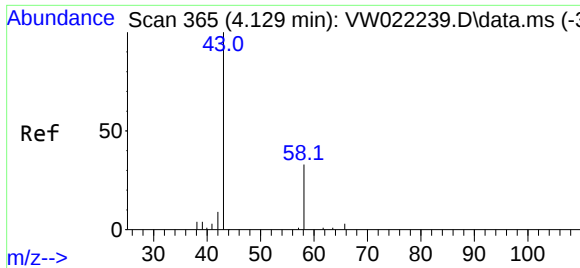

#13
Acetone
Concen: 4.452 ug/L m
RT: 4.129 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW022247.D
Acq: 09 Mar 2022 12:44

Instrument :
MSVOA_W
ClientSampleId :
DBSG6

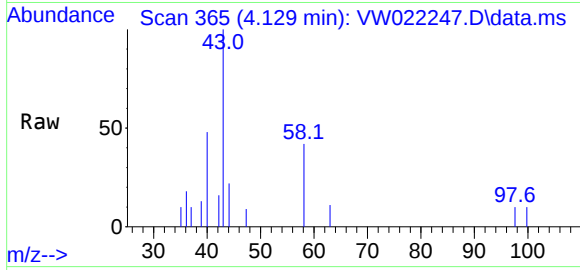

Tgt Ion: 43 Resp: 1534
Ion Ratio Lower Upper
43 100
58 36.5 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

