

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022250.D
 Acq On : 09 Mar 2022 13:56
 Operator : SY/VA
 Sample : N1818-06
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:14:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	153637	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	146420	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	69031	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	53232	26.564	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 106.240%			
7) Chloroethane-d5	2.879	69	33949	21.532	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 86.120%			
11) 1,1-Dichloroethene-d2	4.013	63	50313	16.395	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 65.600%			
21) 2-Butanone-d5	7.080	46	19634	58.274	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 116.540%			
24) Chloroform-d	7.647	84	74411	21.708	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 86.840%			
26) 1,2-Dichloroethane-d4	8.305	65	44369	24.901	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 99.600%			
32) Benzene-d6	8.275	84	149560	21.948	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 87.800%			
36) 1,2-Dichloropropane-d6	9.274	67	40988	21.659	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 86.640%			
41) Toluene-d8	10.323	98	144880	21.385	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 85.560%			
43) trans-1,3-Dichloroprop...	10.579	79	18526	22.079	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 88.320%			
47) 2-Hexanone-d5	10.927	63	15693	50.419	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 100.840%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	40416	24.335	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 97.320%			
66) 1,2-Dichlorobenzene-d4	13.853	152	52931	23.873	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 95.480%			
Target Compounds					Qvalue	
13) Acetone	4.123	43	950m	3.452	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022250.D
Acq On : 09 Mar 2022 13:56
Operator : SY/VA
Sample : N1818-06
Misc : 6.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBSF2

Quant Time: Mar 10 04:14:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022

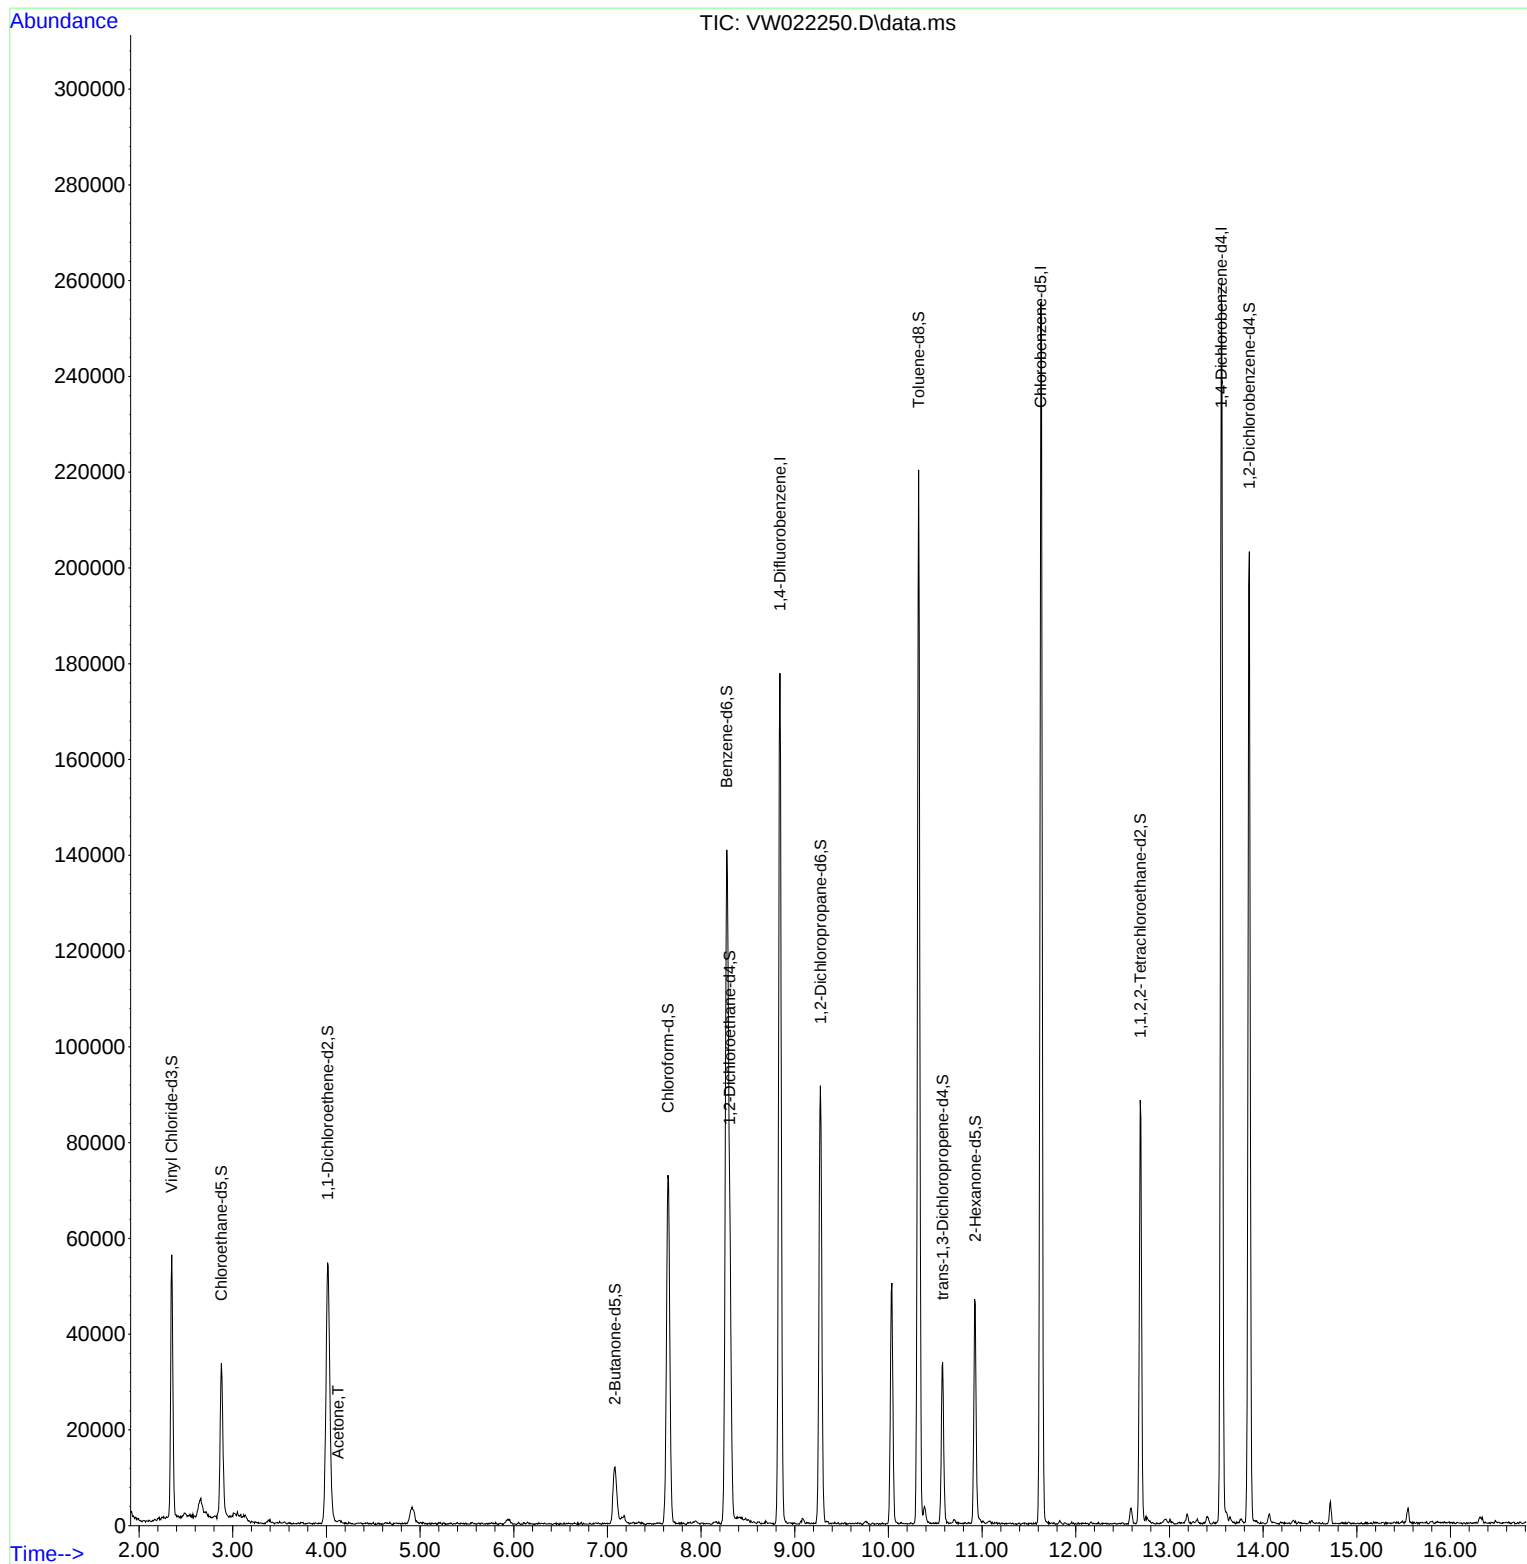

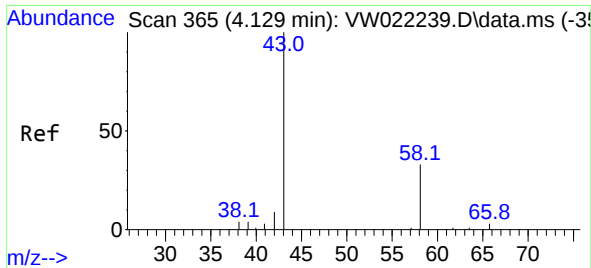

#13
 Acetone
 Concen: 3.452 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW022250.D
 Acq: 09 Mar 2022 13:56

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF2

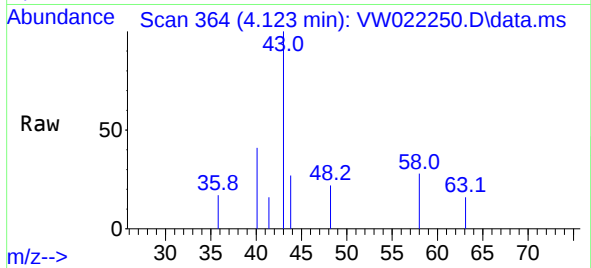

Tgt Ion: 43 Resp: 950
 Ion Ratio Lower Upper
 43 100
 58 17.3 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

