

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022259.D
 Acq On : 09 Mar 2022 17:33
 Operator : SY/VA
 Sample : N1818-05
 Misc : 6.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF1

Quant Time: Mar 10 04:16:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	185837	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	172388	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81639	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	71060	29.317	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	117.280%
7) Chloroethane-d5	2.879	69	44605	23.388	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.560%
11) 1,1-Dichloroethene-d2	4.013	63	67227	18.111	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.440%
21) 2-Butanone-d5	7.080	46	20912	51.313	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.620%
24) Chloroform-d	7.647	84	101800	24.552	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	8.305	65	54456	25.266	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.080%
32) Benzene-d6	8.274	84	202642	25.258	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.040%
36) 1,2-Dichloropropane-d6	9.274	67	55873	25.077	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.320%
41) Toluene-d8	10.323	98	197495	24.760	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.040%
43) trans-1,3-Dichloroprop...	10.579	79	23572	23.861	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.440%
47) 2-Hexanone-d5	10.920	63	16405	44.767	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.540%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	45968	23.509	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	70507	26.889	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.560%
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	7.177	96	5019	2.197	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022259.D
Acq On : 09 Mar 2022 17:33
Operator : SY/VA
Sample : N1818-05
Misc : 6.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSF1


Quant Time: Mar 10 04:16:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

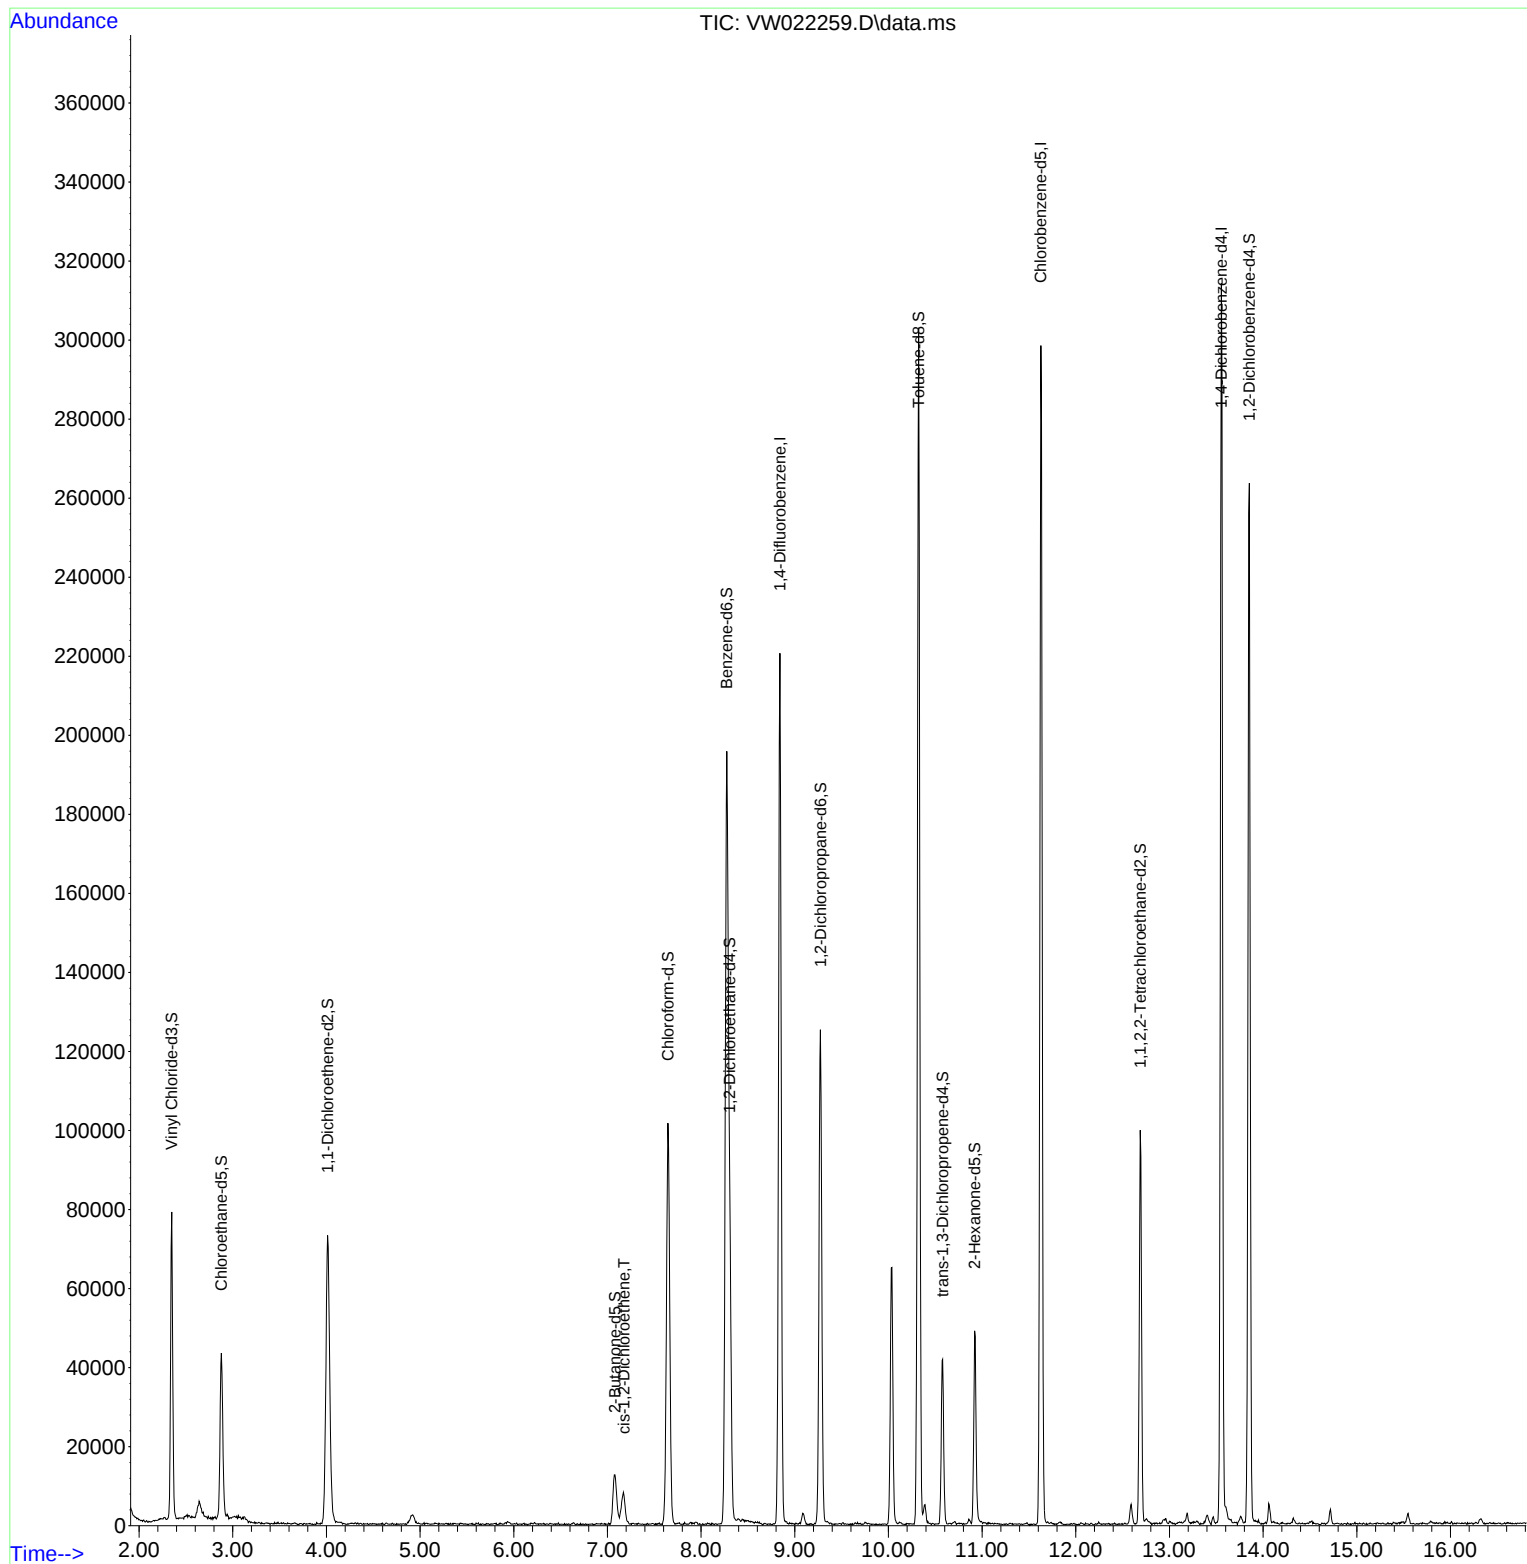

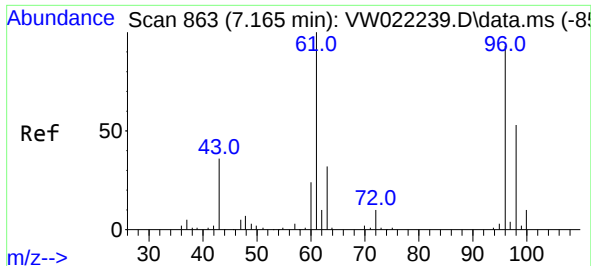

#20
 cis-1,2-Dichloroethene
 Concen: 2.197 ug/L
 RT: 7.177 min Scan# 80
 Delta R.T. 0.012 min
 Lab File: VW022259.D
 Acq: 09 Mar 2022 17:33

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSF1

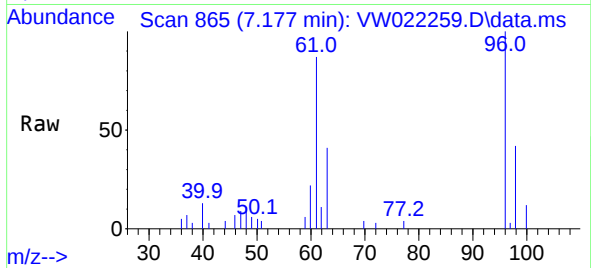

Tgt Ion: 96 Resp: 5019

Ion	Ratio	Lower	Upper
96	100		
61	86.8	76.8	142.6
68	0.0	0.0	0.0

