

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
 Data File : VW022261.D
 Acq On : 09 Mar 2022 18:21
 Operator : SY/VA
 Sample : N1838-02
 Misc : 5.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0QA0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 10 04:16:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 10 04:11:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	143094	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	143476	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	67986	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	49868	26.719	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 106.880%			
7) Chloroethane-d5	2.879	69	33228	22.627	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 90.520%			
11) 1,1-Dichloroethene-d2	4.019	63	50575	17.695	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 70.800%			
21) 2-Butanone-d5	7.074	46	22224	70.821	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 141.640%#			
24) Chloroform-d	7.647	84	78949	24.729	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 98.920%			
26) 1,2-Dichloroethane-d4	8.305	65	47392	28.557	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 114.240%			
32) Benzene-d6	8.275	84	154787	23.181	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 92.720%			
36) 1,2-Dichloropropane-d6	9.275	67	45307	24.433	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 97.720%			
41) Toluene-d8	10.323	98	150062	22.605	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 90.400%			
43) trans-1,3-Dichloroprop...	10.579	79	20278	24.663	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 98.640%			
47) 2-Hexanone-d5	10.921	63	17523	57.454	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 114.900%			
56) 1,1,2,2-Tetrachloroeth...	12.689	84	45217	27.784	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 111.120%			
66) 1,2-Dichlorobenzene-d4	13.853	152	55416	25.378	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 101.520%			
Target Compounds					Qvalue	
13) Acetone	4.123	43	1188m	4.635	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022261.D
Acq On : 09 Mar 2022 18:21
Operator : SY/VA
Sample : N1838-02
Misc : 5.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0QA0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/14/2022


Quant Time: Mar 10 04:16:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 10 04:11:04 2022
Response via : Initial Calibration

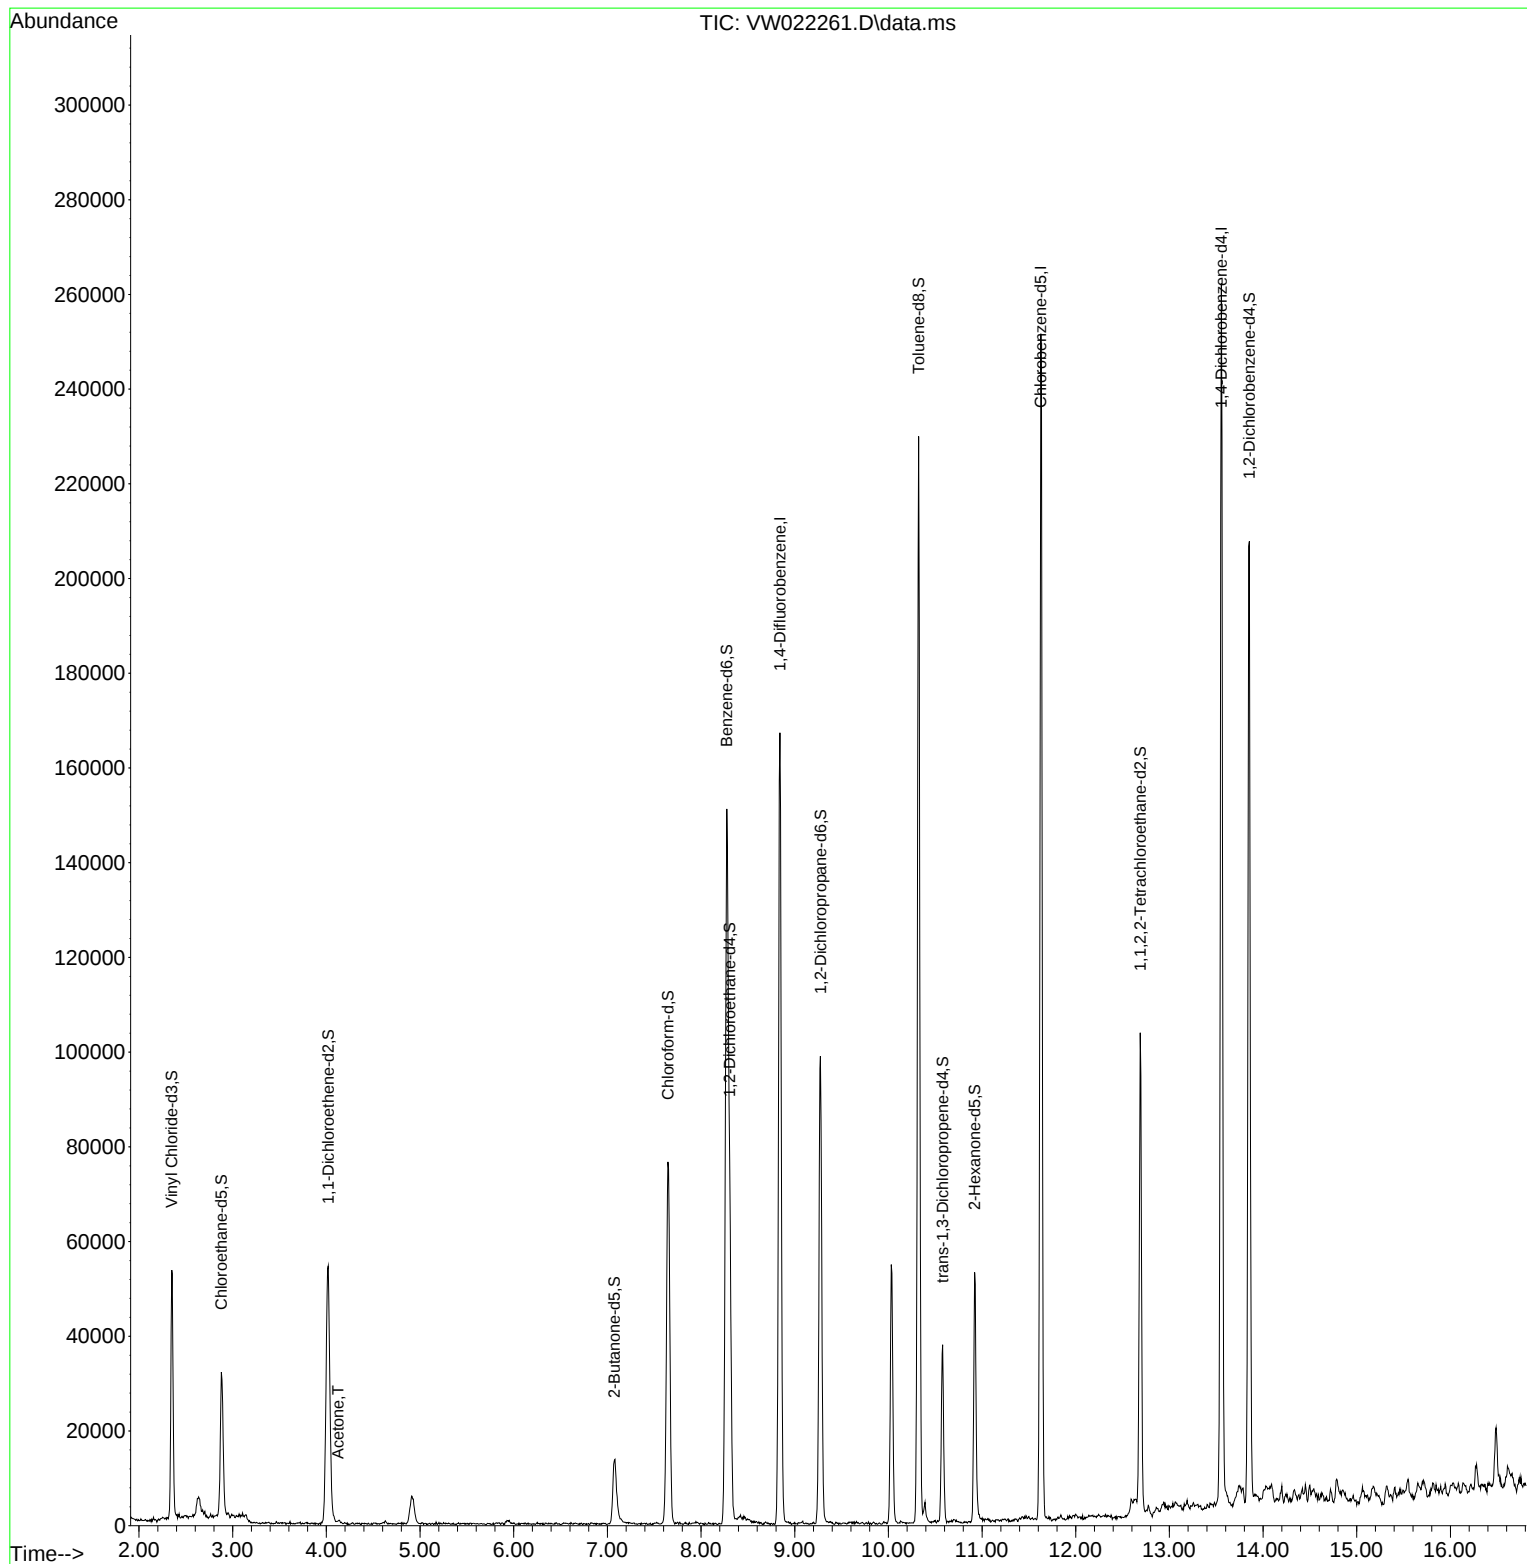

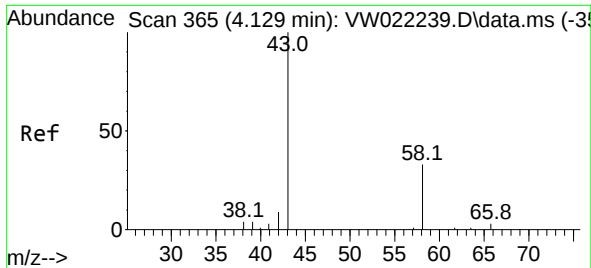

#13
 Acetone
 Concen: 4.635 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW022261.D
 Acq: 09 Mar 2022 18:21

Instrument :
 MSVOA_W
 ClientSampleId :
 C0QA0

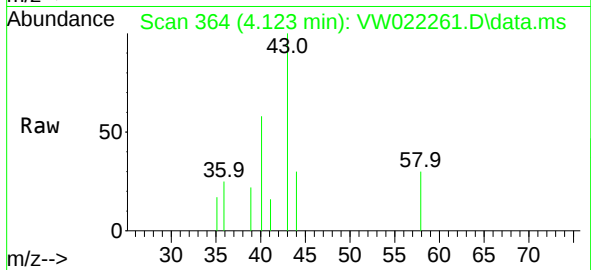

Tgt Ion: 43 Resp: 1188
 Ion Ratio Lower Upper
 43 100
 58 13.8 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/14/2022

