
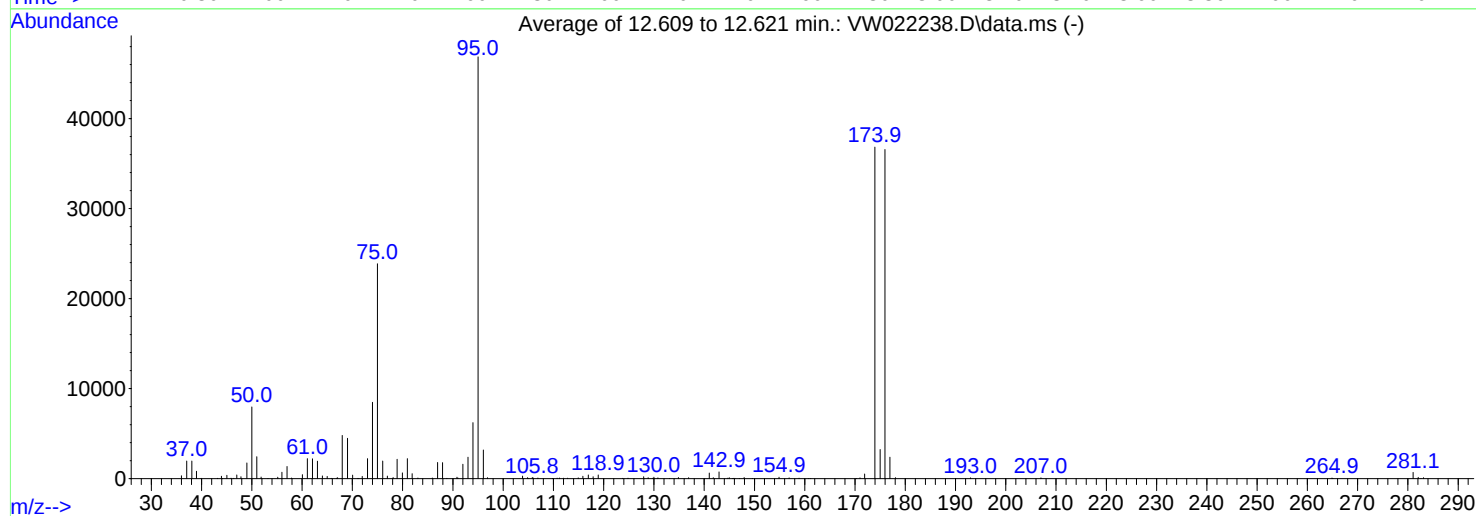


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030922\
Data File : VW022238.D
Acq On : 09 Mar 2022 08:06
Operator : SY/VA
Sample : BFB519
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB519

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Title : SFAM01.0
Last Update : Fri Mar 11 21:01:07 2022

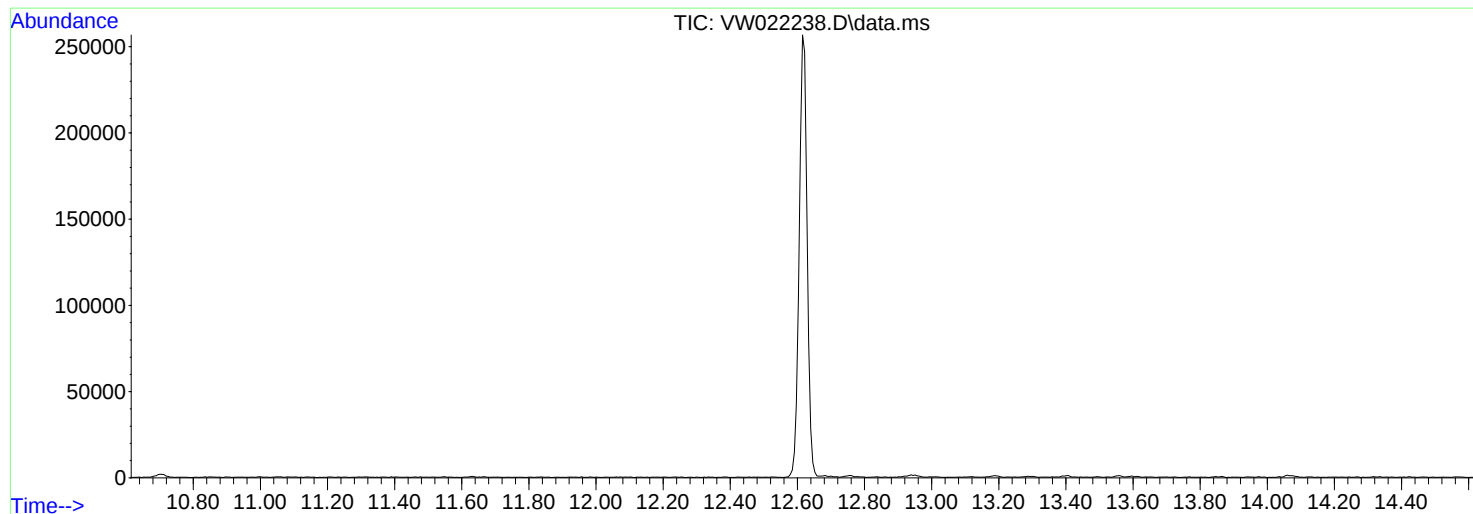

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	7960	PASS
75	95	30	80	50.9	23867	PASS
95	95	100	100	100.0	46864	PASS
96	95	5	9	6.8	3178	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.6	36835	PASS
175	174	5	9	8.8	3239	PASS
176	174	95	105	99.3	36571	PASS
177	176	5	10	6.5	2381	PASS

m/z	Abundance
40.00	177.0
41.20	77.0
44.10	90.0
57.00	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB519

m/z	Abundance
36.00	366.0
37.10	1901.0
38.00	1541.0
39.00	823.0
39.90	186.0
43.20	115.0
44.00	359.0
45.10	332.0
45.80	59.0
47.00	401.0
47.80	236.0
49.00	1611.0
50.00	6951.0
51.00	2413.0
51.80	161.0
53.20	74.0
55.20	99.0
56.00	770.0
57.00	1374.0
57.80	66.0
60.00	355.0
61.10	2231.0
62.00	2031.0
63.00	1671.0
64.10	322.0
65.00	231.0
66.90	139.0
68.00	4128.0
69.00	4027.0
70.10	415.0
71.10	89.0
71.90	194.0
73.00	2046.0
74.00	7227.0
75.00	19936.0
76.00	1833.0
77.00	205.0
78.90	1678.0
80.00	644.0
80.90	2029.0
81.90	532.0
83.00	129.0
85.90	59.0
86.90	1664.0
87.90	1560.0
88.80	97.0
90.80	251.0
92.00	1327.0
93.00	1997.0
94.00	5073.0
95.00	39808.0
96.00	2684.0
96.90	129.0
103.90	265.0
104.80	153.0
105.80	101.0
106.80	77.0
110.80	59.0
111.20	73.0
112.00	61.0
115.00	87.0
115.90	231.0
117.00	385.0
118.00	201.0
118.90	376.0
124.80	53.0
128.00	159.0
128.90	79.0
129.80	187.0
130.80	101.0
133.10	82.0
134.80	75.0
136.80	82.0
141.00	512.0
141.70	89.0
143.00	682.0
144.70	180.0
147.00	76.0
148.00	74.0
149.60	67.0
154.90	144.0
157.00	59.0
171.00	123.0
171.90	535.0
173.90	29128.0
174.90	2477.0
176.00	25968.0
176.90	2096.0
178.10	116.0
193.00	94.0
207.00	85.0
264.90	113.0

Instrument :
MSVOA_W
ClientSampleId :
BFB519

281.00	1007.0
282.00	164.0
283.00	191.0

Instrument :
MSVOA_W
ClientSampleId :
BFB519

m/z	Abundance
36.00	265.0
37.00	2042.0
38.10	2186.0
39.00	861.0
39.90	247.0
43.90	431.0
45.00	414.0
45.90	89.0
46.40	85.0
47.00	446.0
47.90	216.0
49.00	1964.0
50.00	8990.0
51.00	2639.0
51.90	198.0
55.10	202.0
56.00	726.0
57.00	1531.0
57.90	97.0
60.10	524.0
61.00	2317.0
62.10	2347.0
63.10	2361.0
64.10	344.0
65.00	350.0
65.80	67.0
67.10	169.0
68.00	5265.0
69.00	5030.0
70.00	355.0
71.30	67.0
72.00	285.0
73.00	2428.0
74.00	9636.0
75.00	27088.0
76.10	2103.0
76.90	339.0
78.10	171.0
78.90	2550.0
79.90	633.0
81.00	2355.0
81.90	606.0
83.10	81.0
85.80	79.0
87.00	1869.0
87.90	1917.0
90.80	256.0
92.00	1817.0
93.00	2618.0
94.00	6918.0
95.00	53088.0
96.00	3756.0
96.90	127.0
103.80	289.0
105.10	111.0
106.00	217.0
106.90	70.0
110.80	53.0
111.20	54.0
112.00	51.0
112.80	63.0
115.00	64.0
115.80	316.0
116.90	427.0
117.80	212.0
118.90	430.0
123.80	50.0
124.80	68.0
128.00	224.0
128.90	94.0
130.00	286.0
130.80	67.0
134.90	193.0
136.90	128.0
141.00	699.0
141.80	138.0
143.00	803.0
145.00	173.0
145.60	60.0
146.10	127.0
148.00	160.0
154.90	208.0
156.80	95.0
158.90	79.0
171.90	536.0
173.90	38024.0
175.00	3729.0
175.90	40824.0
177.00	2750.0
178.00	93.0
193.00	131.0
207.00	91.0

Instrument :
MSVOA_W
ClientSampleId :
BFB519

264.90	95.0
281.10	681.0
282.00	138.0
282.60	61.0
283.10	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB519

m/z	Abundance
36.00	317.0
37.00	1951.0
38.00	2122.0
39.00	797.0
39.90	220.0
44.20	300.0
45.00	359.0
47.00	391.0
47.90	200.0
49.00	1671.0
50.00	7939.0
51.00	2232.0
51.90	167.0
55.10	165.0
56.00	632.0
57.00	1447.0
58.00	52.0
60.10	435.0
61.00	2145.0
62.00	2242.0
63.00	1794.0
64.00	245.0
65.00	177.0
65.80	62.0
67.00	132.0
68.00	4991.0
69.10	4384.0
70.00	392.0
72.00	255.0
73.00	2209.0
74.00	8574.0
75.00	24576.0
76.10	1948.0
77.00	335.0
78.10	183.0
78.90	2239.0
79.90	665.0
80.90	2276.0
81.90	522.0
86.00	55.0
86.90	1840.0
88.00	1848.0
91.00	235.0
92.00	1644.0
93.00	2540.0
94.00	6668.0
95.00	47696.0
96.10	3093.0
96.90	63.0
103.90	284.0
104.90	166.0
105.80	287.0
107.00	71.0
109.80	57.0
110.70	60.0
111.20	76.0
112.00	52.0
112.90	86.0
114.90	115.0
115.90	254.0
116.90	405.0
117.90	226.0
118.90	414.0
123.80	72.0
124.90	56.0
127.90	236.0
128.80	155.0
130.00	170.0
130.80	80.0
134.80	102.0
137.00	131.0
141.00	655.0
141.90	99.0
142.80	742.0
145.00	168.0
145.80	132.0
147.80	136.0
154.90	147.0
156.90	104.0
158.80	61.0
160.80	56.0
161.20	54.0
170.30	58.0
171.00	122.0
171.90	452.0
174.00	43352.0
175.10	3510.0
175.90	42920.0
176.90	2296.0
178.00	104.0
193.10	68.0
207.00	75.0

Instrument :
MSVOA_W
ClientSampleId :
BFB519

265.10	54.0
281.10	391.0
282.10	123.0
283.20	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB519