


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW031020\
 Data File : VW015106.D
 Acq On : 10 Mar 2020 10:12
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030920S.M
 Title : SW846 8260
 Last Update : Mon Mar 09 18:51:48 2020

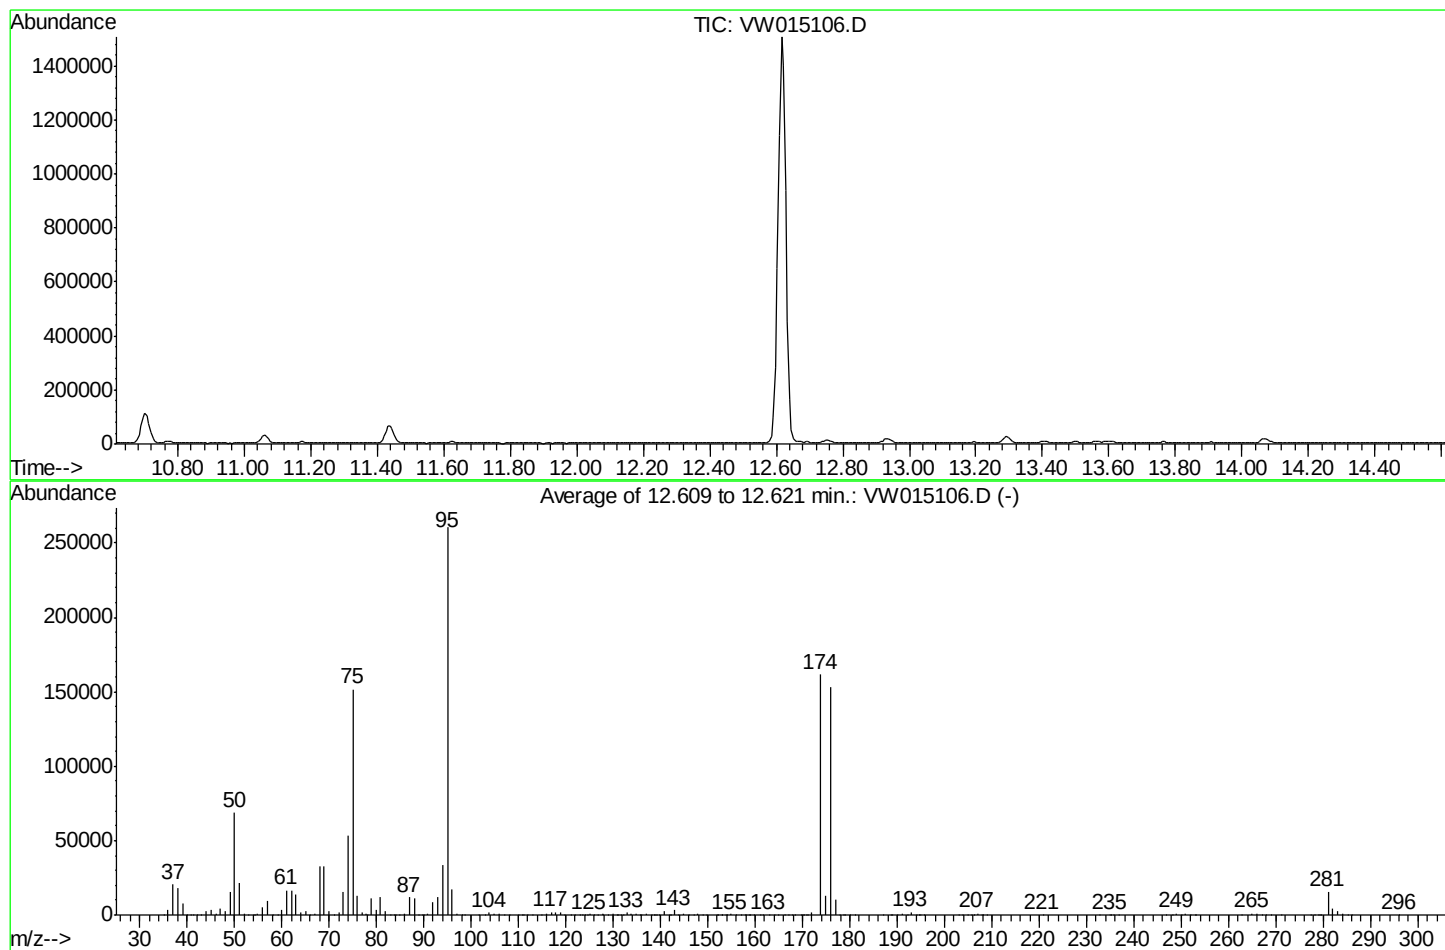

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.3	68616	PASS
75	95	30	60	58.1	151461	PASS
95	95	100	100	100.0	260522	PASS
96	95	5	9	6.7	17437	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	62.0	161485	PASS
175	174	5	9	8.2	13227	PASS
176	174	95	101	94.9	153272	PASS
177	176	5	9	6.9	10650	PASS