

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031021\
 Data File : VW018290.D
 Acq On : 10 Mar 2021 16:05
 Operator : SY/VA
 Sample : VIBLK12
 Misc : 6.23G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK12

Manual Integrations
 APPROVED

MMDadoda
 3/15/2021 12:37:47 PM

Quant Time: Mar 11 02:04:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 11 02:01:11 2021
 Response via : Initial Calibration

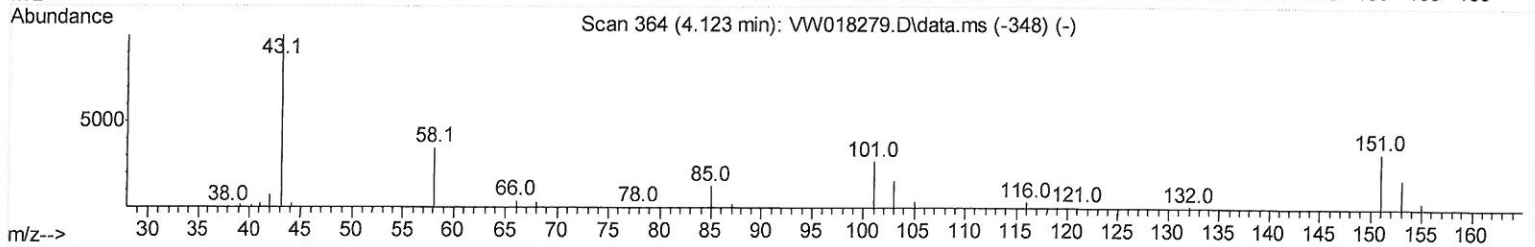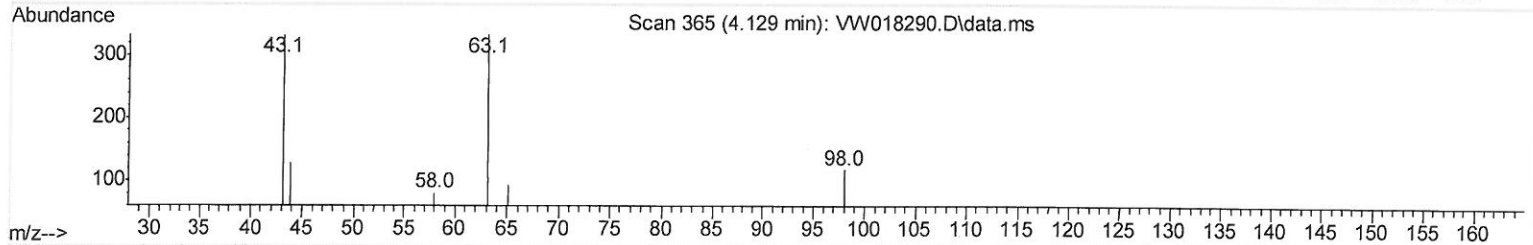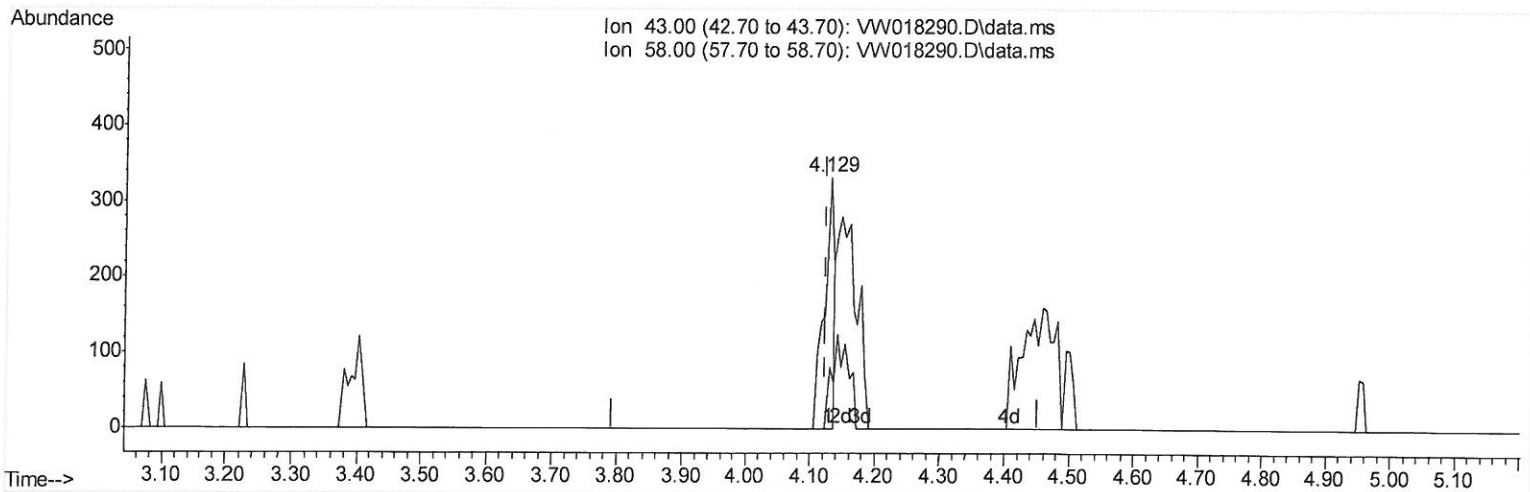

TIC: VW018290.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 0.63 ug/L

response 345

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031021\
 Data File : VW018290.D
 Acq On : 10 Mar 2021 16:05
 Operator : SY/VA
 Sample : VIBLK12
 Misc : 6.23G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK12

Manual Integrations
 APPROVED

MMDadoda
 3/15/2021 12:37:47 PM

Quant Time: Mar 11 02:04:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 11 02:01:11 2021
 Response via : Initial Calibration

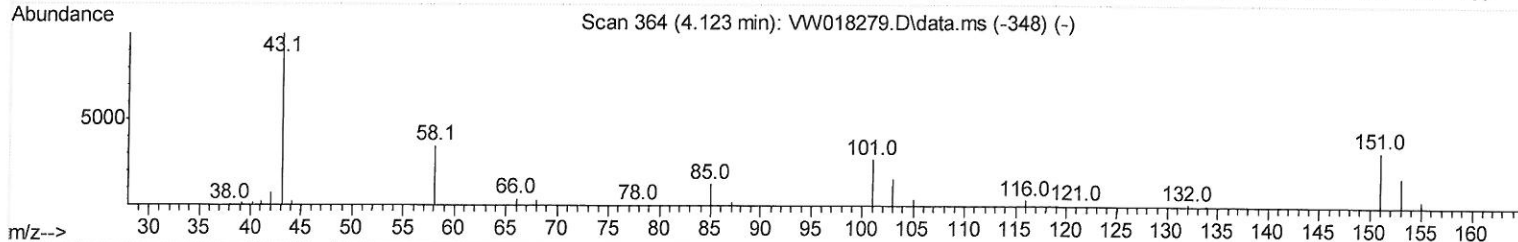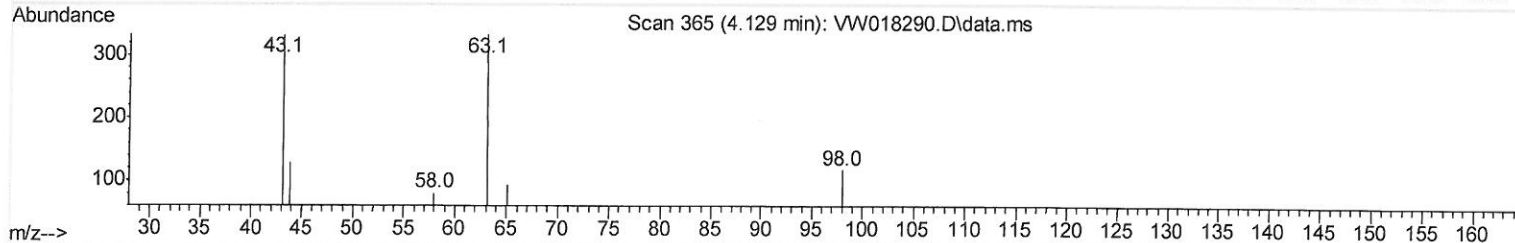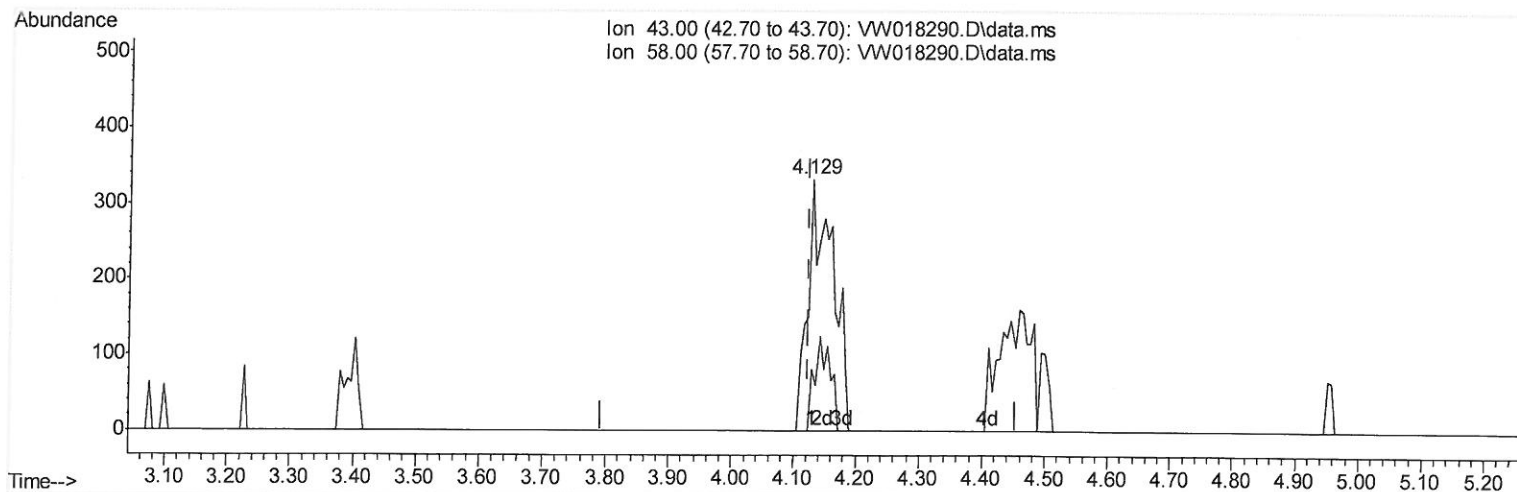

TIC: VW018290.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 1.70 ug/L m

response 936

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031021\
 Data File : VW018290.D
 Acq On : 10 Mar 2021 16:05
 Operator : SY/VA
 Sample : VIBLK12
 Misc : 6.23G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK12

Manual Integrations
 APPROVED

MMDadoda
 3/15/2021 12:37:47 PM

Quant Time: Mar 11 02:04:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 11 02:01:11 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	273292	25.00	ug/L	0.00
28) Chlorobenzene-d5		11.634	117	250959	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4		13.560	152	114392	25.00	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.361	65	77205	26.09	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150		Recovery	=	104.36%	
7) Chloroethane-d5		2.891	69	59216	24.64	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150		Recovery	=	98.56%	
10) 1,1-Dichloroethene-d2		4.019	63	124221	18.06	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110		Recovery	=	72.24%	
20) 2-Butanone-d5		7.080	46	29226	41.54	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135		Recovery	=	83.08%	
24) Chloroform-d		7.653	84	171202	23.12	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150		Recovery	=	92.48%	
26) 1,2-Dichloroethane-d4		8.305	65	96222	23.61	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130		Recovery	=	94.44%	
29) Benzene-d6		8.275	84	319590	23.92	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135		Recovery	=	95.68%	
33) 1,2-Dichloropropane-d6		9.274	67	87149	23.54	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120		Recovery	=	94.16%	
37) Toluene-d8		10.323	98	308710	23.94	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130		Recovery	=	95.76%	
38) trans-1,3-Dichloroprop...		10.579	79	40406	22.02	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135		Recovery	=	88.08%	
39) 2-Hexanone-d5		10.927	63	25984	42.19	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135		Recovery	=	84.38%	
48) 1,1,2,2-Tetrachloroeth...		12.688	84	69661	22.01	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120		Recovery	=	88.04%	
61) 1,2-Dichlorobenzene-d4		13.853	152	97281	23.40	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120		Recovery	=	93.60%	
Target Compounds							Qvalue
13) Acetone		4.129	43	936m	1.70	ug/L	03
16) Methylene chloride		4.922	84	26387	6.33	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031021\
Data File : VW018290.D
Acq On : 10 Mar 2021 16:05
Operator : SY/VA
Sample : VIBLK12
Misc : 6.23G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VIBLK12

Manual Integrations
APPROVED

MMDadoda
3/15/2021 12:37:47 PM

Quant Time: Mar 11 02:04:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 11 02:01:11 2021
Response via : Initial Calibration

