

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031021\
 Data File : VW018288.D
 Acq On : 10 Mar 2021 15:17
 Operator : SY/VA
 Sample : VIBLK11
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK11

Quant Time: Mar 11 02:04:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 11 02:01:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	257728	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	231318	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	108953	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	79155	28.36	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 113.44%			
7) Chloroethane-d5	2.897	69	62076	27.39	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 109.56%			
10) 1,1-Dichloroethene-d2	4.025	63	126009	19.43	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 77.72%			
20) 2-Butanone-d5	7.074	46	32890	49.57	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 99.14%			
24) Chloroform-d	7.647	84	182220	26.10	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 104.40%			
26) 1,2-Dichloroethane-d4	8.305	65	98422	25.61	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 102.44%			
29) Benzene-d6	8.275	84	333741	27.10	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 108.40%			
33) 1,2-Dichloropropane-d6	9.274	67	91384	26.78	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 107.12%			
37) Toluene-d8	10.323	98	323544	27.23	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 108.92%			
38) trans-1,3-Dichloroprop...	10.579	79	42750	25.28	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 101.12%			
39) 2-Hexanone-d5	10.920	63	28619	50.42	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 100.84%			
48) 1,1,2,2-Tetrachloroeth...	12.688	84	72898	24.98	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 99.92%			
61) 1,2-Dichlorobenzene-d4	13.853	152	103453	26.12	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 104.48%			
Target Compounds						Qvalue
16) Methylene chloride	4.921	84	9906	2.52	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031021\
Data File : VW018288.D
Acq On : 10 Mar 2021 15:17
Operator : SY/VA
Sample : VIBLK11
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK11

Quant Time: Mar 11 02:04:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 11 02:01:11 2021
Response via : Initial Calibration

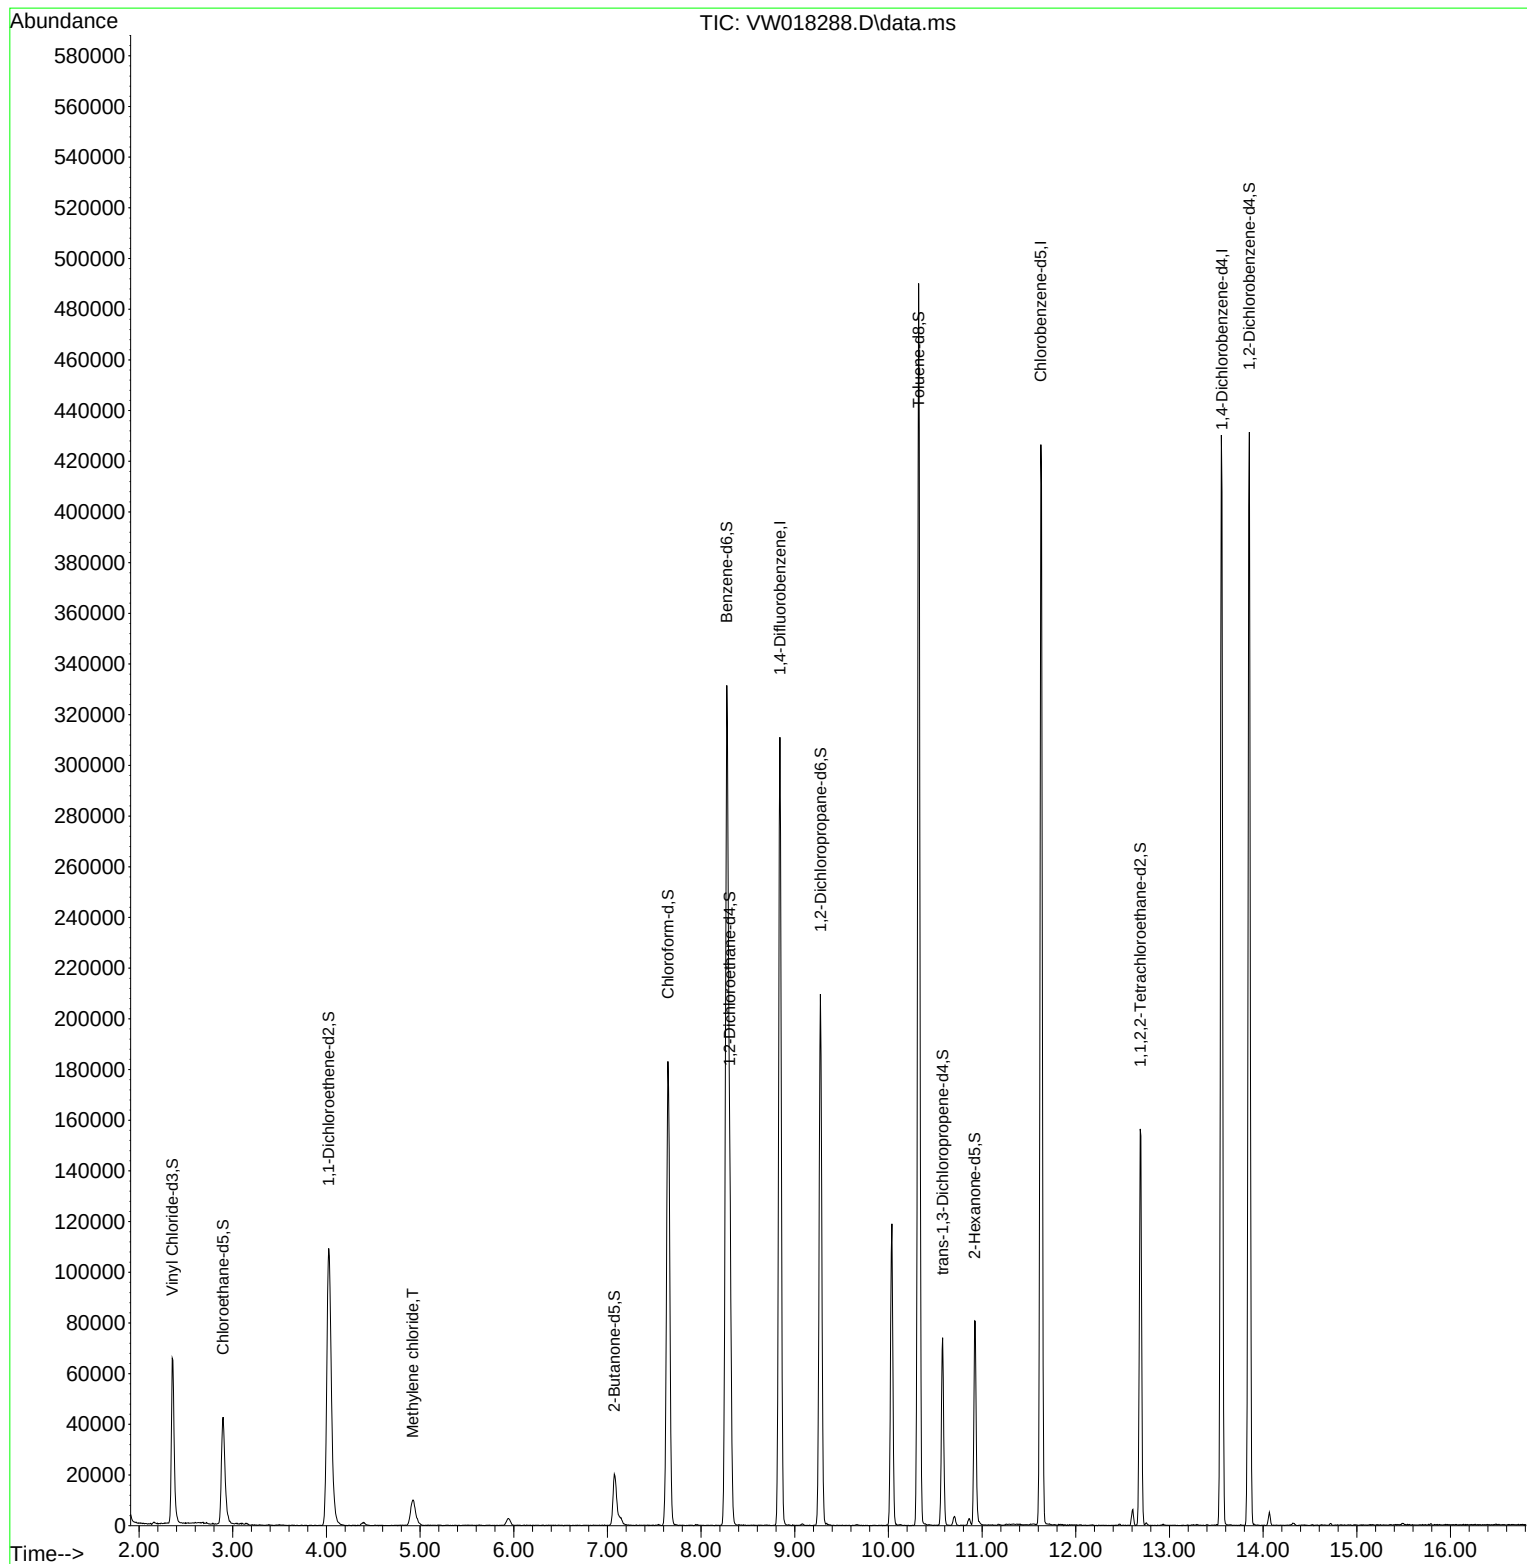

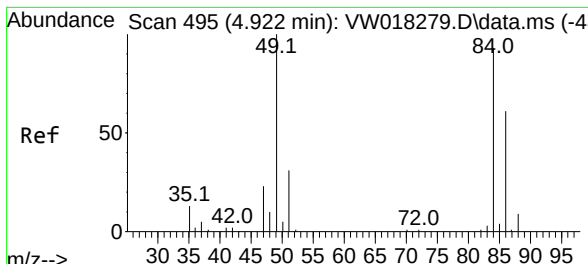

#16
Methylene chloride
Concen: 2.52 ug/L
RT: 4.921 min Scan# 495
Delta R.T. -0.000 min
Lab File: VW018288.D
Acq: 10 Mar 2021 15:17

Instrument :
MSVOA_W
ClientSampleId :
VIBLK11

Tgt Ion:	84	Resp:	9906
Ion	Ratio	Lower	Upper
84	100		
49	99.5	74.4	138.2
86	59.7	46.1	85.7

