
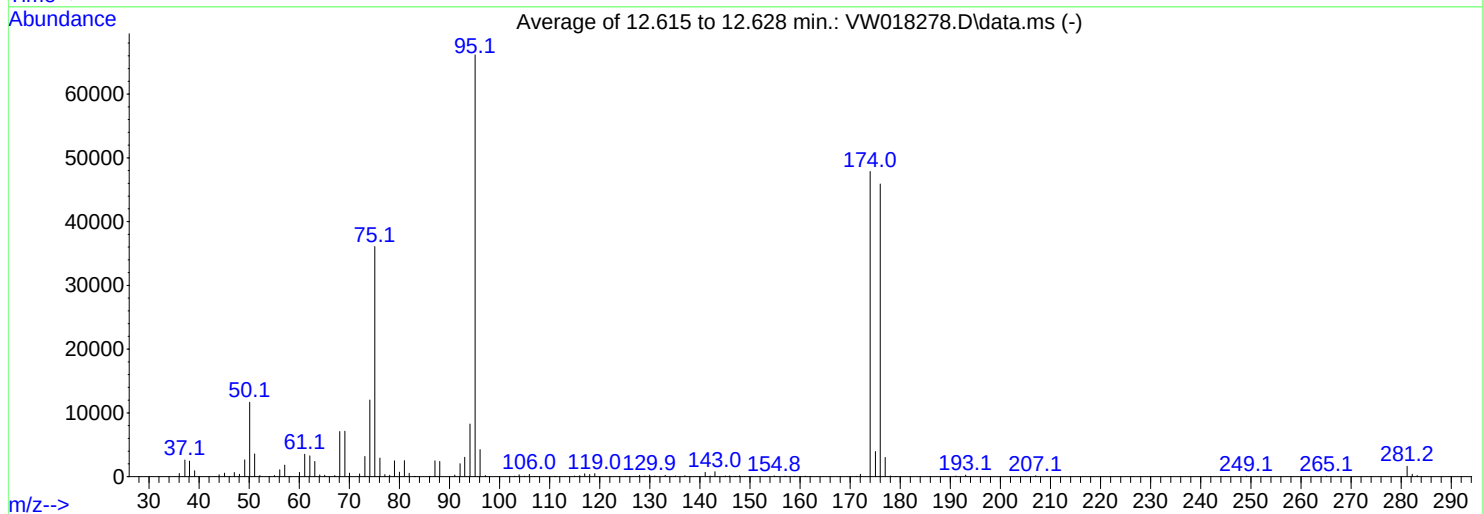


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031021\
 Data File : VW018278.D
 Acq On : 10 Mar 2021 09:09
 Operator : SY/VA
 Sample : BFB12
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB12

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Title : VOC Analysis
 Last Update : Thu Mar 11 02:01:11 2021

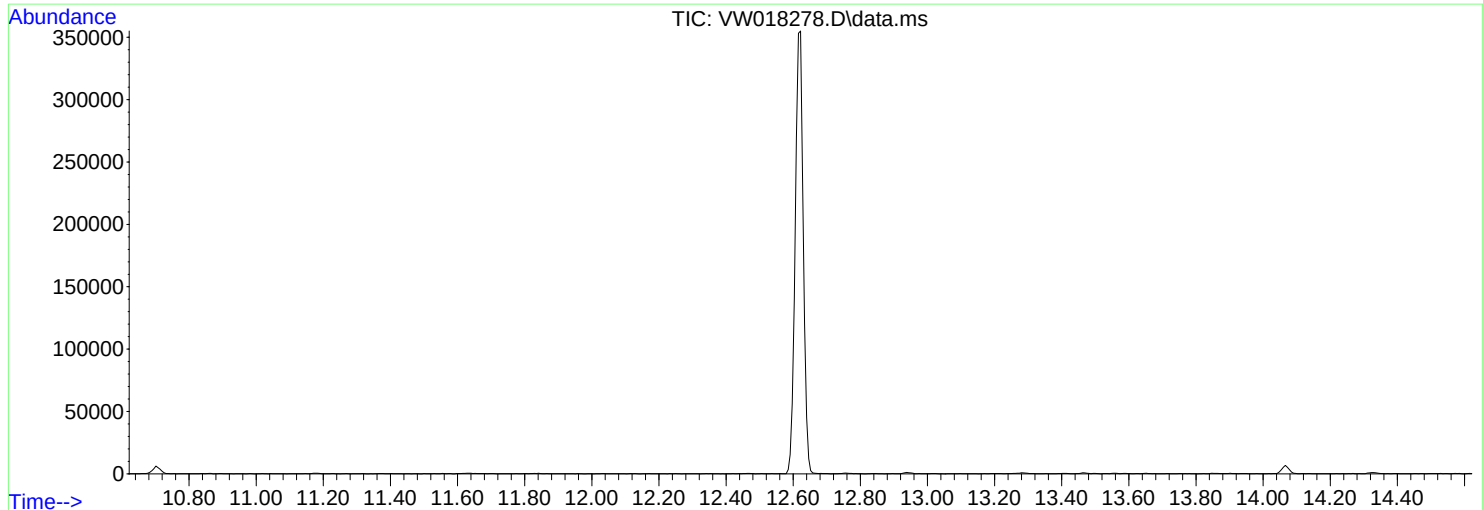

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	11672	PASS
75	95	30	80	54.5	36077	PASS
95	95	100	100	100.0	66155	PASS
96	95	5	9	6.4	4255	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.3	47861	PASS
175	174	5	9	8.2	3930	PASS
176	174	95	101	95.9	45901	PASS
177	176	5	9	6.5	3005	PASS

m/z	Abundance
36.10	620.0
37.10	3045.0
38.10	2975.0
39.10	1067.0
40.10	119.0
44.10	482.0
45.10	808.0
46.20	77.0
47.00	803.0
48.10	468.0
49.10	3221.0
50.10	14097.0
51.10	4338.0
52.10	241.0
55.00	204.0
56.10	1374.0
57.10	2192.0
58.00	70.0
60.10	830.0
61.10	4455.0
62.10	3858.0
63.10	3006.0
64.10	384.0
65.10	282.0
67.20	225.0
68.10	8168.0
69.10	8911.0
70.10	593.0
72.00	462.0
73.10	3405.0
74.10	14305.0
75.10	41336.0
76.10	3439.0
77.20	350.0
78.00	234.0
79.00	3084.0
80.00	814.0
81.00	2738.0
82.00	575.0
83.00	54.0
86.00	86.0
87.10	2668.0
88.10	2598.0
91.00	273.0
92.10	2507.0
93.00	3732.0
94.10	9850.0
95.10	73872.0
96.10	4910.0
97.20	186.0
103.00	116.0
103.90	404.0
105.00	74.0
106.00	424.0
107.00	116.0
110.00	71.0
111.00	59.0
113.00	96.0
114.90	167.0
115.90	293.0
117.10	558.0
118.00	391.0
119.00	625.0
123.90	53.0
125.20	110.0
126.00	57.0
127.90	161.0
129.00	125.0
129.90	271.0
131.00	179.0
133.10	384.0
134.20	64.0
135.20	135.0
136.90	112.0
141.10	675.0
142.10	153.0
143.00	899.0
145.10	236.0
146.00	145.0
147.00	83.0
147.90	183.0
148.90	84.0
154.90	151.0
157.00	92.0
159.00	91.0
161.00	98.0
171.20	165.0
172.10	374.0
174.00	45792.0
175.00	4022.0
176.00	47752.0
177.00	3410.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

178.00	69.0
179.10	61.0
191.10	238.0
193.10	360.0
194.10	57.0
205.10	71.0
207.00	280.0
208.00	62.0
249.10	171.0
265.10	185.0
281.20	2806.0
282.20	511.0
283.20	382.0
284.10	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

m/z	Abundance
36.00	584.0
37.10	2806.0
38.10	2746.0
39.10	1128.0
40.10	135.0
44.10	430.0
45.10	473.0
46.10	64.0
47.10	729.0
48.10	334.0
49.10	2896.0
50.10	12462.0
51.10	3657.0
52.20	199.0
55.00	203.0
56.10	1281.0
57.10	1941.0
58.00	113.0
60.10	671.0
61.10	3741.0
62.10	3544.0
63.10	2618.0
64.00	304.0
65.10	261.0
67.00	218.0
68.10	7721.0
69.10	7094.0
70.00	607.0
72.10	541.0
73.10	3795.0
74.10	12931.0
75.10	41272.0
76.10	3369.0
77.10	416.0
78.10	256.0
79.00	2582.0
80.00	789.0
81.00	2874.0
81.90	656.0
83.00	82.0
86.00	93.0
87.10	3025.0
88.00	2969.0
91.10	317.0
92.10	2178.0
93.10	3203.0
94.10	8740.0
95.10	74536.0
96.10	4904.0
97.10	227.0
103.10	79.0
103.90	293.0
105.00	71.0
105.90	318.0
106.90	64.0
110.00	54.0
111.00	104.0
115.00	120.0
116.10	220.0
116.90	483.0
118.00	398.0
118.90	438.0
125.20	73.0
128.00	250.0
129.00	117.0
130.00	277.0
131.00	147.0
133.00	184.0
134.80	109.0
135.20	89.0
137.00	249.0
141.00	869.0
142.00	65.0
143.00	814.0
145.10	98.0
145.90	128.0
147.20	67.0
147.90	206.0
150.00	92.0
154.80	106.0
156.90	108.0
159.00	90.0
161.10	65.0
172.00	507.0
174.00	56048.0
175.10	4341.0
176.00	52480.0
177.00	3393.0
178.00	157.0
191.10	84.0
193.00	286.0
207.10	145.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

249.10	93.0
251.20	58.0
265.10	78.0
281.20	1203.0
282.20	391.0
283.20	171.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

m/z	Abundance
36.00	290.0
37.20	1972.0
38.10	1572.0
39.10	623.0
40.10	85.0
44.00	329.0
45.20	410.0
47.10	424.0
48.00	310.0
49.10	1828.0
50.10	8458.0
51.10	2725.0
52.10	97.0
55.10	144.0
56.10	623.0
57.10	1304.0
58.30	69.0
60.00	565.0
61.10	2376.0
62.10	2397.0
63.10	1551.0
64.20	166.0
65.10	140.0
66.90	58.0
68.10	5375.0
69.10	5410.0
70.00	445.0
72.00	255.0
73.10	2297.0
74.10	8835.0
75.10	25624.0
76.10	1928.0
77.00	237.0
78.00	194.0
79.00	1803.0
80.00	508.0
81.00	1905.0
81.90	380.0
83.20	54.0
86.20	64.0
87.10	1734.0
88.00	1575.0
91.00	192.0
92.10	1392.0
93.00	2192.0
94.10	6214.0
95.10	50056.0
96.10	2950.0
97.20	111.0
103.90	237.0
105.00	79.0
106.00	322.0
111.20	52.0
114.90	59.0
116.00	195.0
117.00	297.0
117.90	201.0
119.10	406.0
128.00	180.0
129.00	75.0
129.90	213.0
133.20	73.0
135.00	70.0
137.10	111.0
141.00	514.0
142.00	65.0
143.00	651.0
144.80	56.0
146.00	127.0
147.10	59.0
148.10	171.0
150.20	64.0
154.90	113.0
157.20	123.0
158.90	74.0
161.10	71.0
172.00	279.0
174.00	41744.0
175.10	3427.0
176.00	37472.0
177.10	2212.0
178.00	72.0
193.10	119.0
207.20	63.0
281.10	853.0
282.20	222.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

m/z	Abundance
40.10	73.0
44.00	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12