
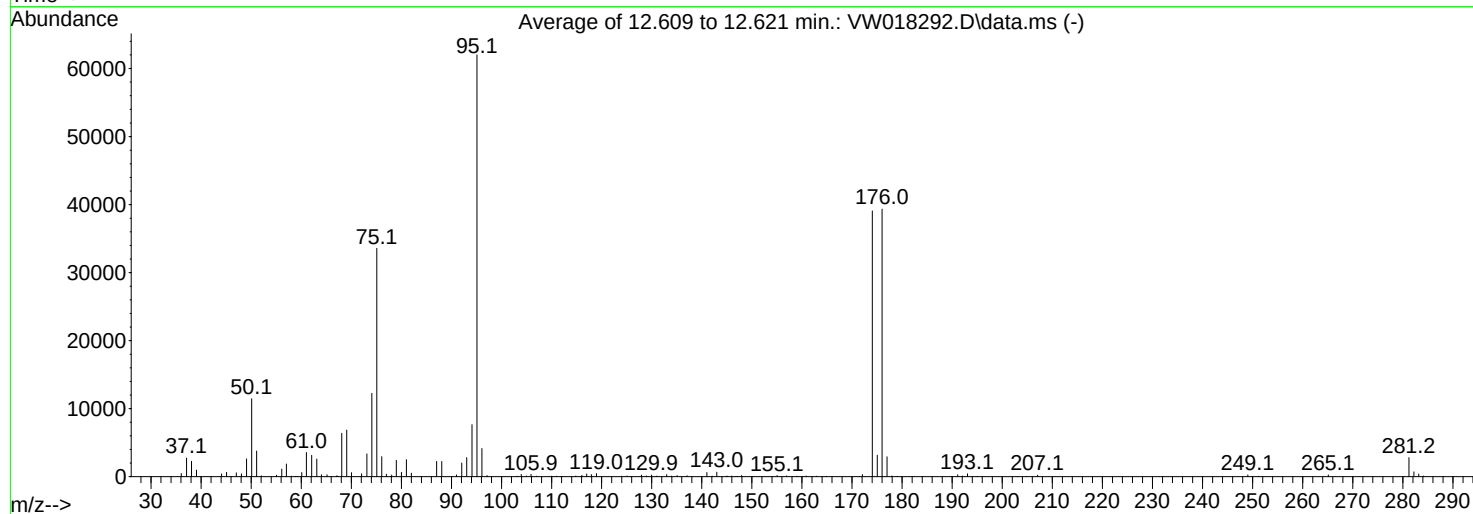


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031121\
Data File : VW018292.D
Acq On : 11 Mar 2021 08:29
Operator : SY/VA
Sample : BFB13
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB13

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
Title : VOC Analysis
Last Update : Sat Mar 13 00:38:12 2021

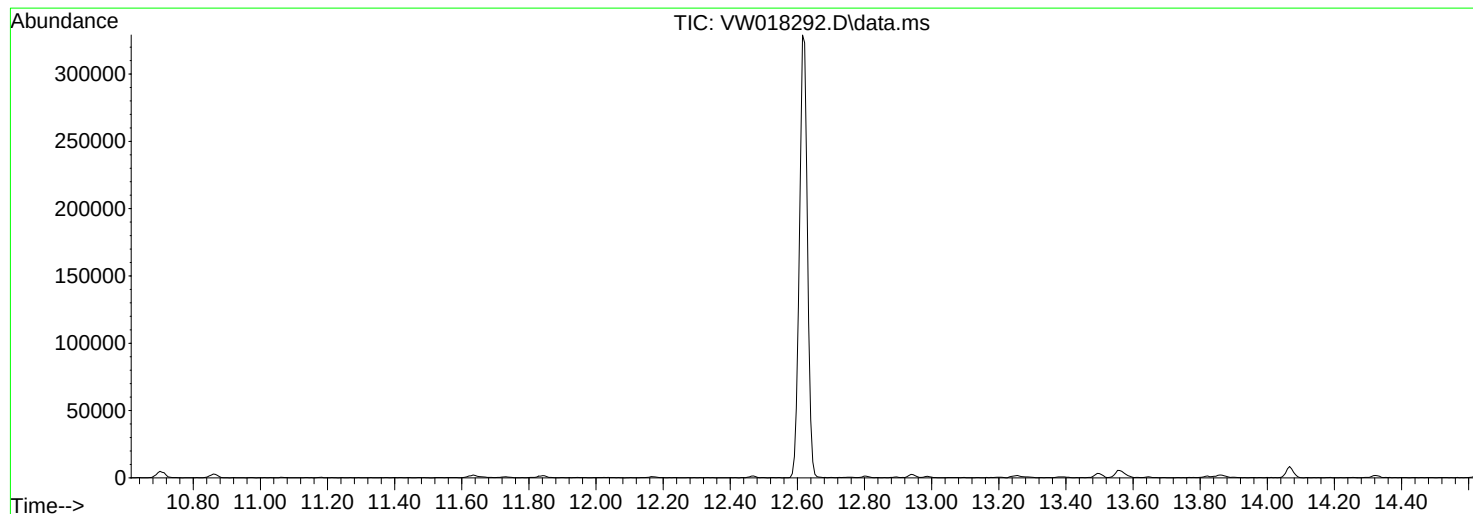

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	11462	PASS
75	95	30	80	54.1	33568	PASS
95	95	100	100	100.0	62013	PASS
96	95	5	9	6.7	4131	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.0	39072	PASS
175	174	5	9	8.1	3163	PASS
176	174	95	101	100.7	39339	PASS
177	176	5	9	7.4	2915	PASS

m/z	Abundance
36.10	370.0
37.10	2479.0
38.10	2044.0
39.10	814.0
40.00	132.0
44.00	464.0
45.10	631.0
46.10	77.0
47.10	433.0
48.00	319.0
49.10	2170.0
50.10	9795.0
51.10	3176.0
52.00	71.0
55.00	212.0
56.10	885.0
57.10	1364.0
58.00	65.0
58.90	122.0
60.10	553.0
61.10	3098.0
62.10	2470.0
63.10	2319.0
64.00	256.0
65.10	248.0
67.10	100.0
68.10	4954.0
69.10	5450.0
70.10	487.0
72.00	296.0
73.10	2777.0
74.10	10664.0
75.10	26784.0
76.10	2505.0
77.00	279.0
77.80	119.0
78.20	170.0
79.00	1988.0
80.00	516.0
81.00	2146.0
82.00	369.0
87.00	1810.0
88.10	1601.0
91.00	187.0
92.00	1424.0
93.00	2168.0
94.10	5722.0
95.10	46728.0
96.10	3417.0
97.10	149.0
103.10	127.0
104.00	205.0
105.10	127.0
106.00	188.0
107.00	82.0
110.00	87.0
111.00	91.0
114.90	100.0
115.90	147.0
117.00	387.0
118.00	314.0
119.00	350.0
124.00	78.0
125.10	148.0
127.90	176.0
129.00	139.0
130.00	162.0
131.00	91.0
133.00	471.0
133.90	94.0
135.00	135.0
137.10	96.0
141.00	489.0
142.00	65.0
143.00	590.0
144.90	96.0
145.90	90.0
146.80	72.0
147.90	124.0
149.90	70.0
155.00	109.0
156.90	98.0
160.80	73.0
162.90	77.0
164.90	90.0
172.00	275.0
174.10	25208.0
175.10	2356.0
176.00	29944.0
177.00	2512.0
178.00	77.0
179.00	140.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

191.10	412.0
192.10	64.0
193.10	639.0
194.00	150.0
195.10	68.0
203.00	55.0
204.90	57.0
207.10	307.0
249.00	268.0
251.20	108.0
265.10	237.0
281.20	3143.0
282.20	998.0
283.20	320.0
284.20	179.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

m/z	Abundance
36.10	553.0
37.10	3091.0
38.10	2460.0
39.10	1087.0
40.00	112.0
44.10	496.0
45.10	682.0
47.10	703.0
48.10	489.0
49.10	3065.0
50.10	12658.0
51.10	4297.0
52.10	137.0
55.00	252.0
56.10	1220.0
57.00	2189.0
58.10	114.0
59.30	99.0
60.10	779.0
61.10	3938.0
62.10	3687.0
63.10	2913.0
64.10	370.0
65.10	270.0
67.10	248.0
68.10	7162.0
69.10	7836.0
70.00	683.0
72.10	457.0
73.10	3774.0
74.10	12992.0
75.10	38344.0
76.10	3266.0
77.00	512.0
78.00	294.0
79.00	2683.0
80.00	580.0
81.00	2842.0
82.00	654.0
87.10	2535.0
88.00	2407.0
91.00	251.0
92.10	2420.0
93.00	3148.0
94.10	8460.0
95.10	70488.0
96.10	4929.0
97.10	251.0
103.10	112.0
103.90	334.0
104.90	77.0
105.90	296.0
107.00	52.0
110.00	111.0
111.00	94.0
111.80	94.0
114.80	99.0
116.10	276.0
116.90	462.0
117.90	302.0
119.00	531.0
123.90	55.0
125.00	105.0
125.80	68.0
127.90	332.0
128.90	104.0
129.90	245.0
131.10	85.0
133.00	279.0
133.90	116.0
135.10	191.0
137.00	137.0
141.00	734.0
142.10	79.0
143.00	675.0
145.10	167.0
146.00	115.0
147.10	64.0
148.00	155.0
155.00	153.0
157.00	135.0
159.00	120.0
160.90	99.0
162.90	112.0
165.00	86.0
172.00	374.0
174.00	45792.0
175.10	3295.0
176.00	39608.0
177.00	3074.0
178.00	75.0
191.10	311.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

192.00	104.0
193.00	431.0
194.90	65.0
203.00	55.0
204.90	71.0
207.00	184.0
249.10	267.0
251.10	59.0
265.10	369.0
281.20	3312.0
282.20	655.0
283.10	633.0
284.10	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

m/z	Abundance
36.00	476.0
37.10	2617.0
38.10	2263.0
39.10	1005.0
40.10	121.0
44.20	468.0
45.10	607.0
47.00	552.0
48.00	376.0
49.10	2572.0
50.10	11933.0
51.10	3795.0
52.10	135.0
55.10	199.0
56.10	1219.0
57.10	2057.0
60.10	516.0
61.00	3644.0
62.10	3207.0
63.10	2560.0
64.10	251.0
65.20	305.0
67.30	208.0
68.10	6995.0
69.10	7275.0
70.10	634.0
72.10	531.0
73.10	3485.0
74.10	13081.0
75.10	35576.0
76.10	3076.0
77.10	249.0
78.00	223.0
79.00	2504.0
80.00	830.0
81.00	2468.0
82.00	561.0
87.10	2386.0
88.00	2684.0
91.00	310.0
92.10	2163.0
93.10	3090.0
94.10	8743.0
95.10	68824.0
96.10	4047.0
97.10	95.0
104.00	454.0
105.00	98.0
105.90	492.0
107.00	58.0
112.10	89.0
114.80	91.0
116.00	322.0
117.10	341.0
118.00	336.0
118.90	435.0
123.90	65.0
125.10	66.0
128.00	216.0
128.90	136.0
130.00	316.0
131.10	98.0
133.10	151.0
134.00	58.0
135.00	169.0
137.00	170.0
141.00	605.0
142.10	99.0
143.00	738.0
145.00	100.0
146.00	89.0
147.10	72.0
147.90	191.0
155.10	210.0
156.90	119.0
159.00	90.0
160.90	111.0
171.50	64.0
172.10	304.0
174.00	46216.0
175.00	3837.0
176.00	48464.0
177.00	3160.0
177.90	130.0
191.00	161.0
192.10	93.0
193.10	207.0
207.10	120.0
249.10	227.0
265.10	139.0
281.10	1920.0
282.10	494.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

283.10

179.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

m/z	Abundance
40.00	96.0
44.20	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13