




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022290.D
 Acq On : 11 Mar 2022 11:16
 Operator : SY/VA
 Sample : N1819-04
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX6

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:02:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

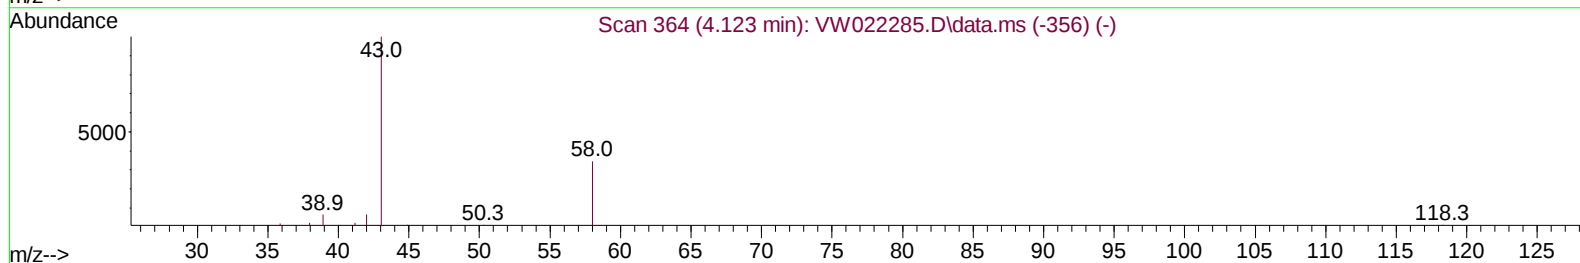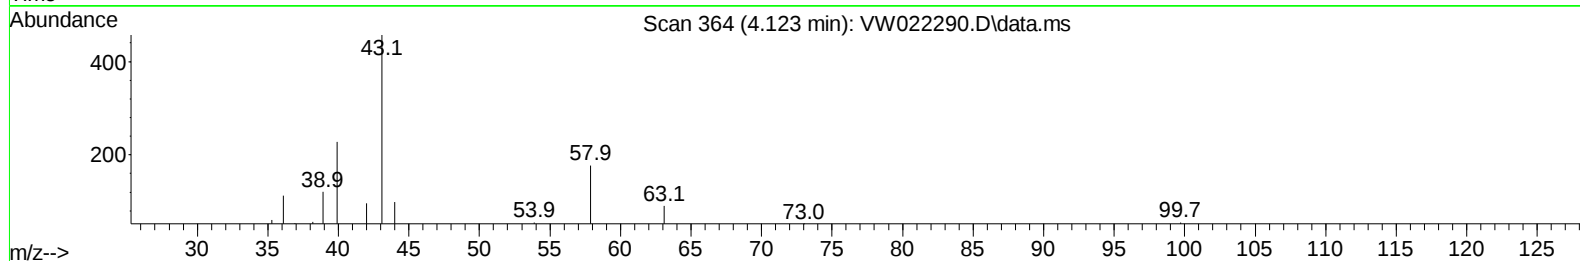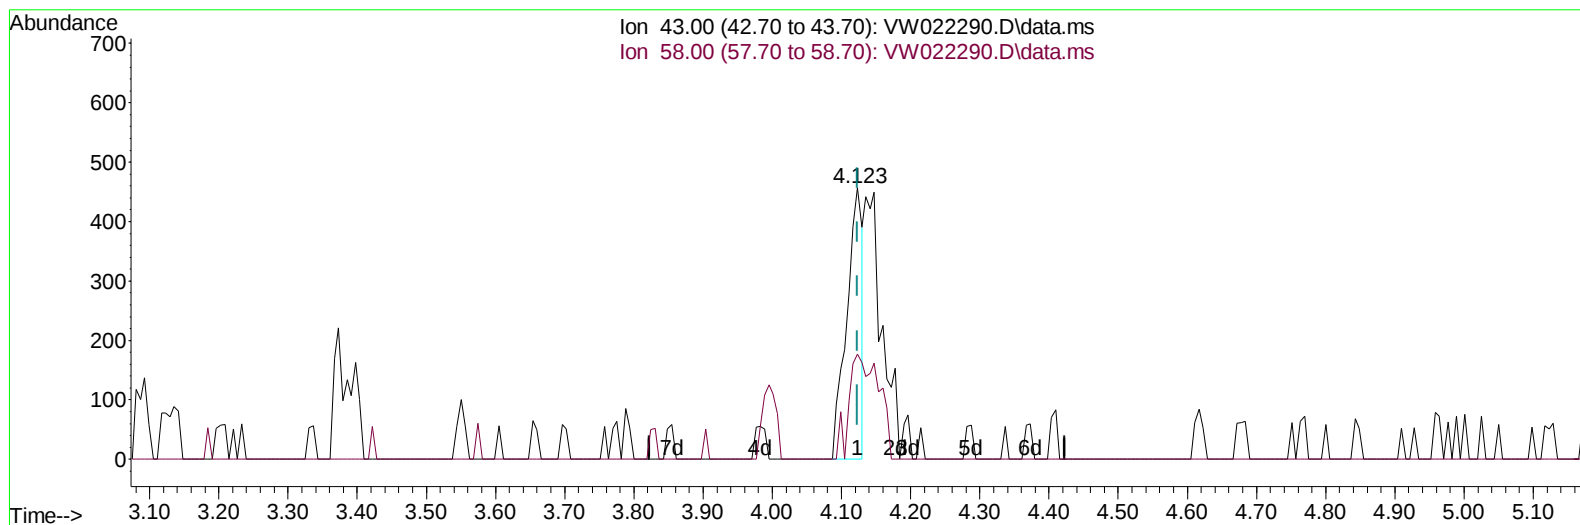

TIC: VW022290.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 2.14 ug/L

response 713

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	37.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022290.D
 Acq On : 11 Mar 2022 11:16
 Operator : SY/VA
 Sample : N1819-04
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX6

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:02:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

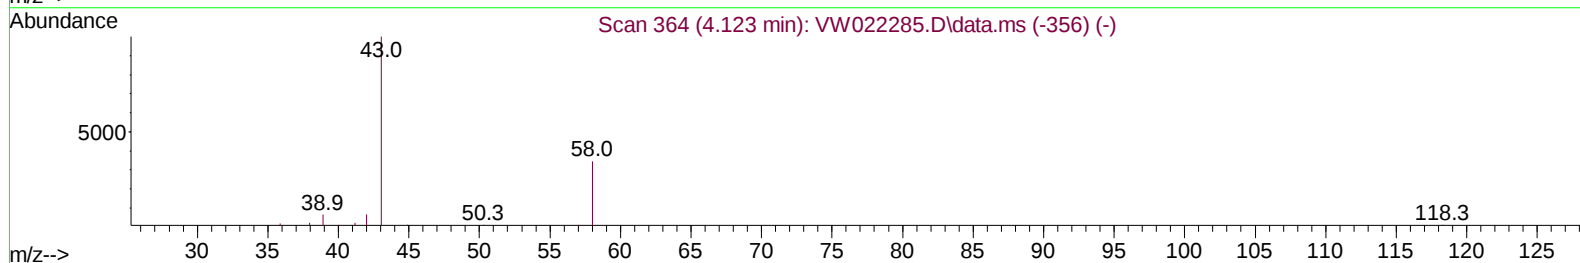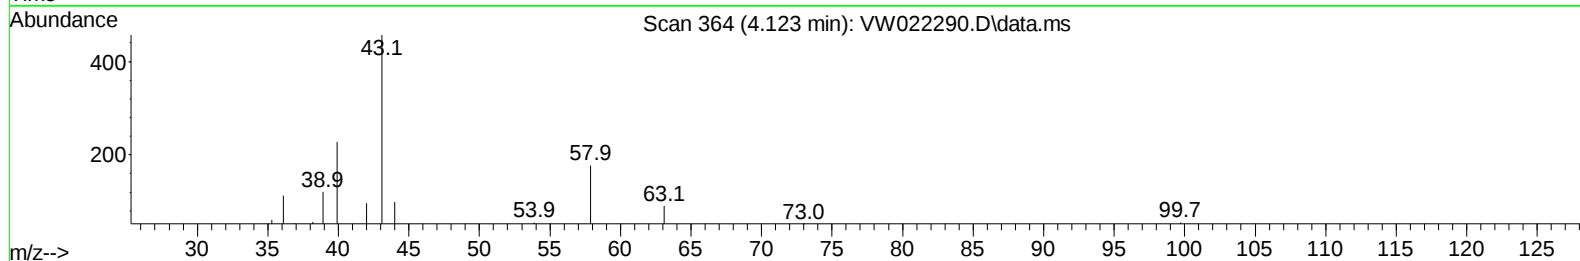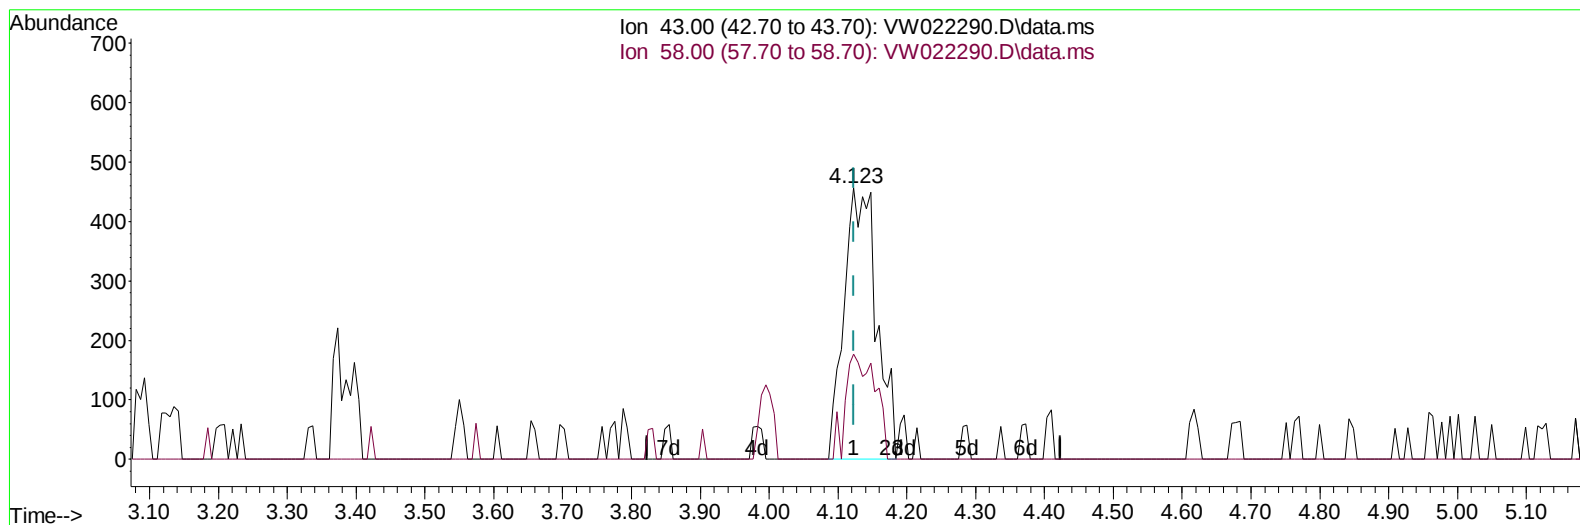

TIC: VW022290.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 4.50 ug/L m

response 1498

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	18.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022290.D
 Acq On : 11 Mar 2022 11:16
 Operator : SY/VA
 Sample : N1819-04
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX6

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:02:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	185750	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	167916	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80443	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	67581	27.894	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	111.560%	
7) Chloroethane-d5	2.879	69	44740	23.470	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	93.880%	
11) 1,1-Dichloroethene-d2	4.013	63	66972	18.051	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	72.200%	
21) 2-Butanone-d5	7.074	46	17924	44.001	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	88.000%	
24) Chloroform-d	7.647	84	103891	25.068	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	100.280%	
26) 1,2-Dichloroethane-d4	8.305	65	51199	23.766	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	95.080%	
32) Benzene-d6	8.275	84	203496	26.040	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	104.160%	
36) 1,2-Dichloropropane-d6	9.275	67	55709	25.669	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.680%	
41) Toluene-d8	10.323	98	196452	25.286	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	101.160%	
43) trans-1,3-Dichloroprop...	10.573	79	21529	22.373	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.480%	
47) 2-Hexanone-d5	10.921	63	14267	39.970	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	79.940%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	41863	21.979	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	87.920%	
66) 1,2-Dichlorobenzene-d4	13.853	152	65787	25.462	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	101.840%	
Target Compounds						
13) Acetone	4.123	43	1498m	4.503	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022290.D
Acq On : 11 Mar 2022 11:16
Operator : SY/VA
Sample : N1819-04
Misc : 5.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRX6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:02:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

