




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022293.D
 Acq On : 11 Mar 2022 12:29
 Operator : SY/VA
 Sample : N1819-07
 Misc : 4.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX7

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:03:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

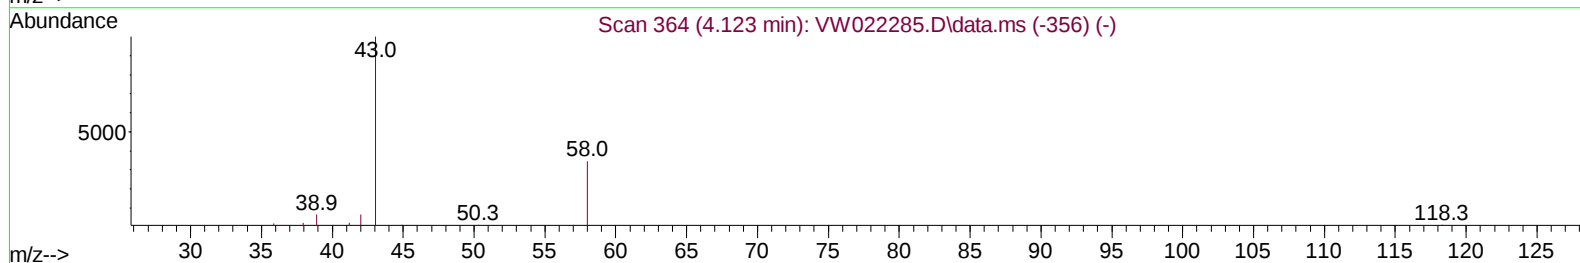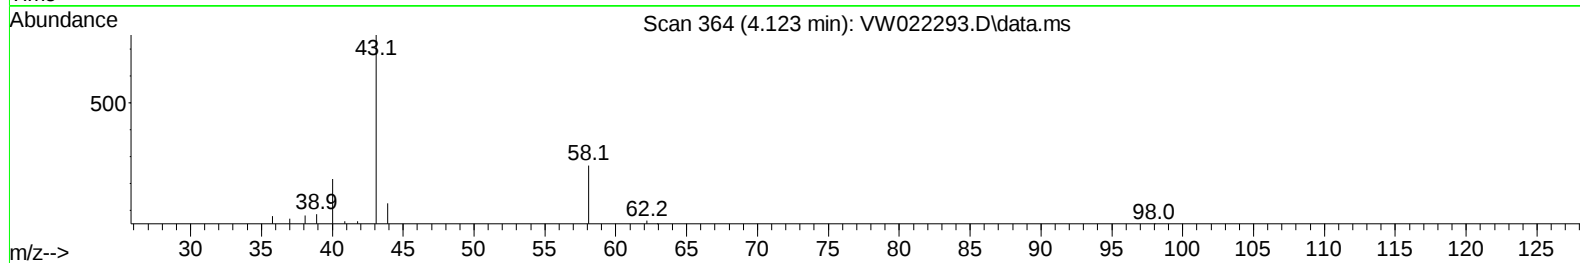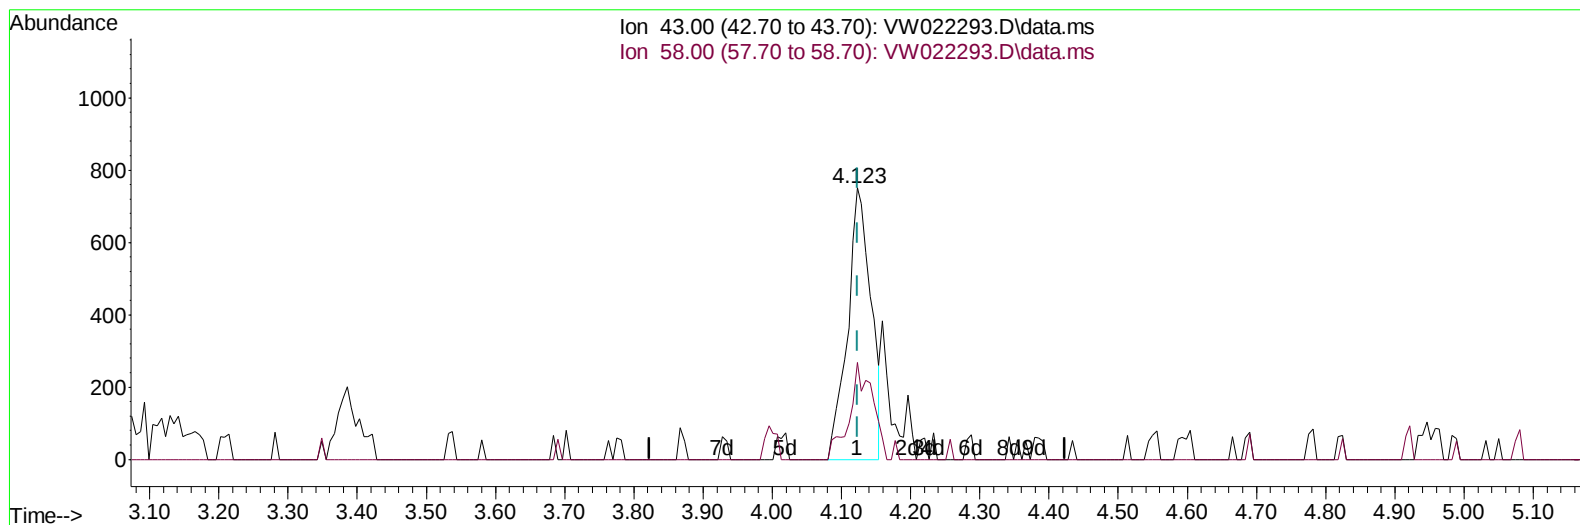

TIC: VW022293.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 5.33 ug/L

response 1754

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	16.13
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022293.D
 Acq On : 11 Mar 2022 12:29
 Operator : SY/VA
 Sample : N1819-07
 Misc : 4.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX7

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:03:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

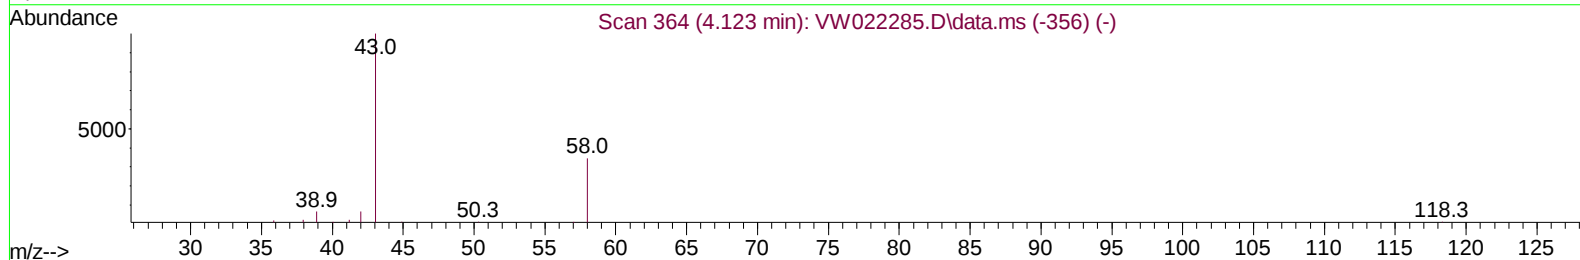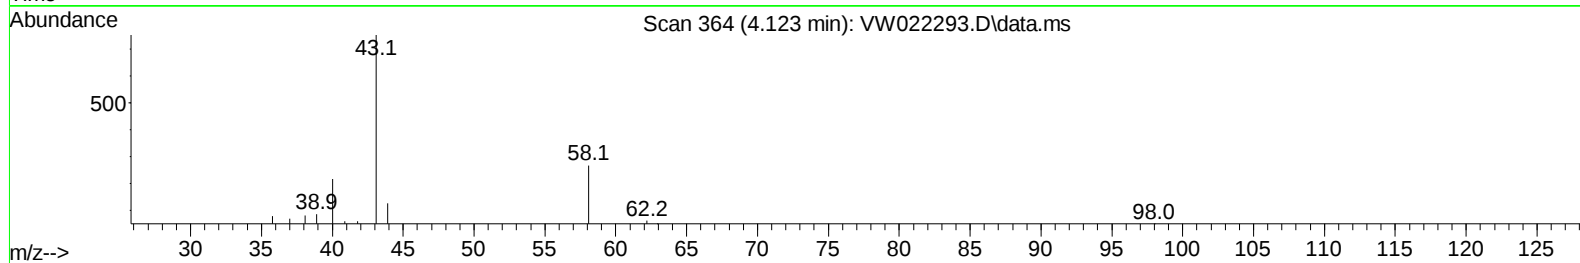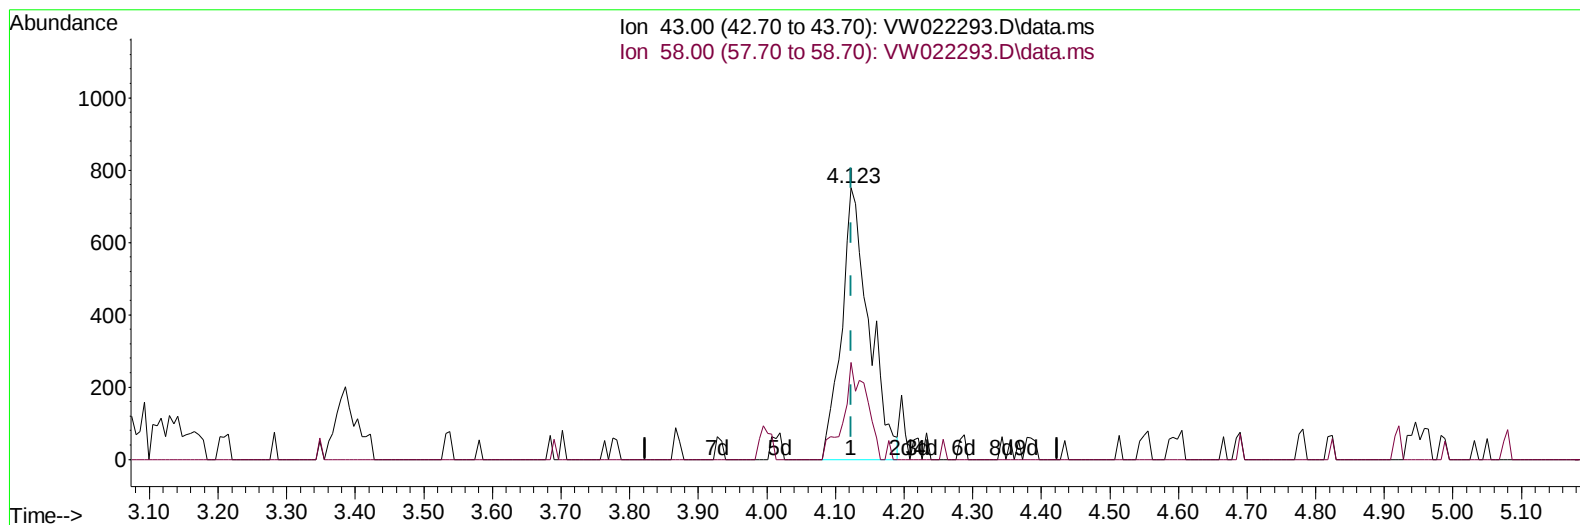

TIC: VW022293.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 6.37 ug/L m

response 2095

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	13.51
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022293.D
Acq On : 11 Mar 2022 12:29
Operator : SY/VA
Sample : N1819-07
Misc : 4.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRX7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:03:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

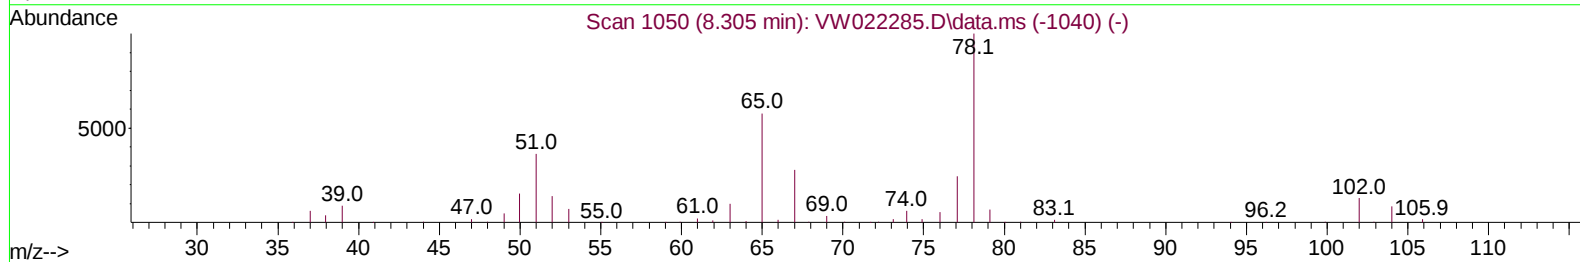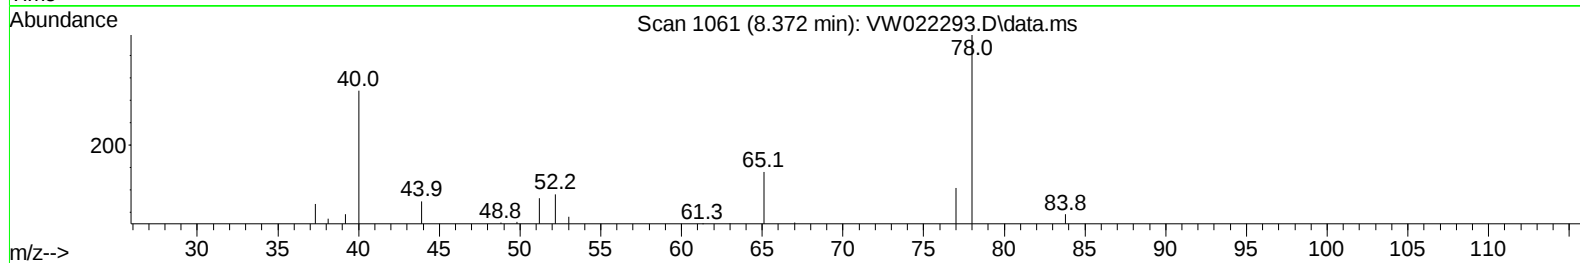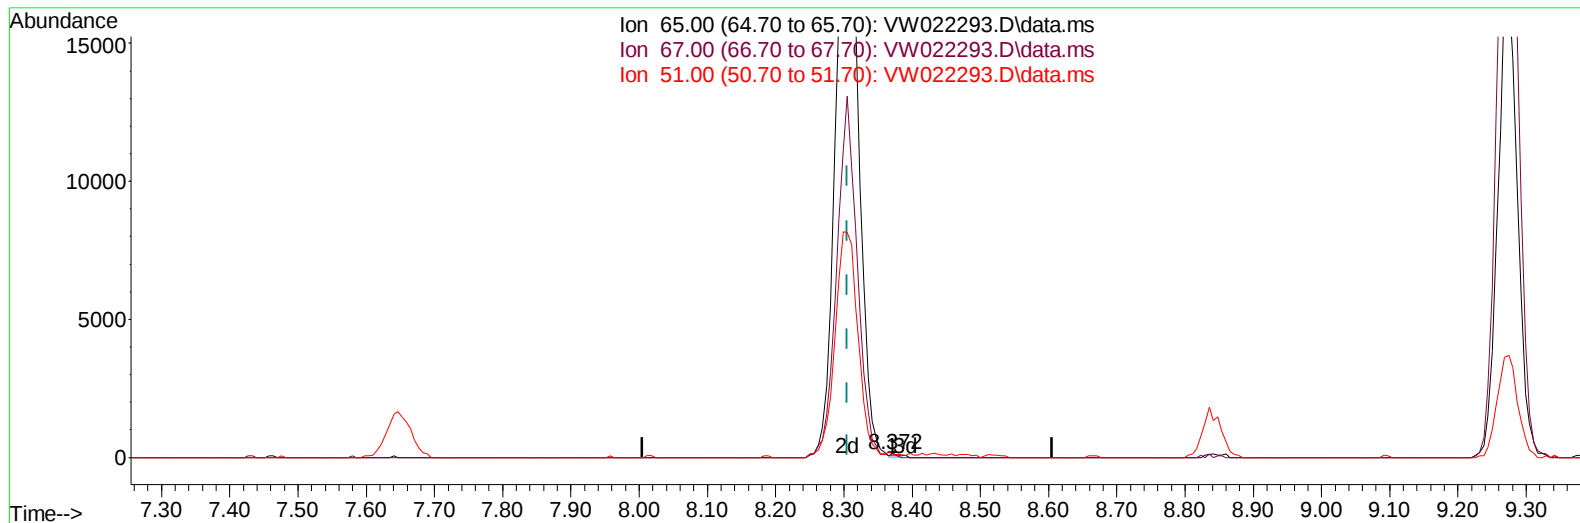

TIC: VW022293.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.372min (+ 0.067) 0.05 ug/L

response 101

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	41.58
51.00	90.00	69.31
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022293.D
 Acq On : 11 Mar 2022 12:29
 Operator : SY/VA
 Sample : N1819-07
 Misc : 4.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:03:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

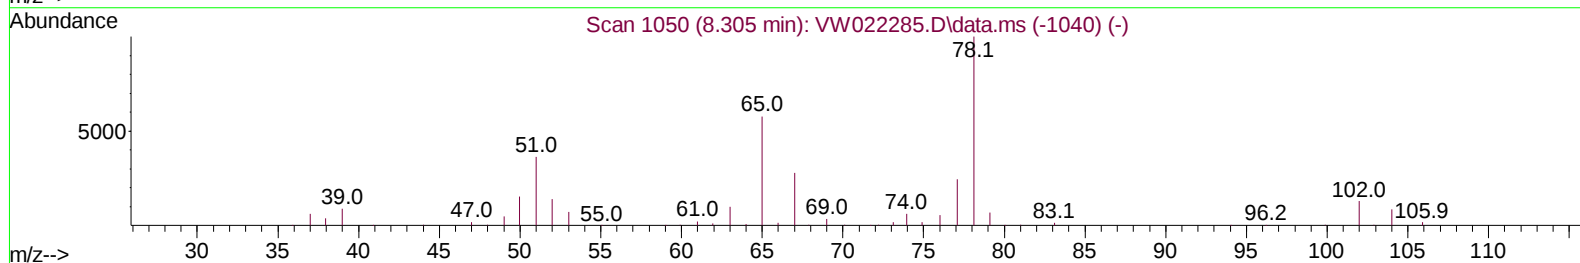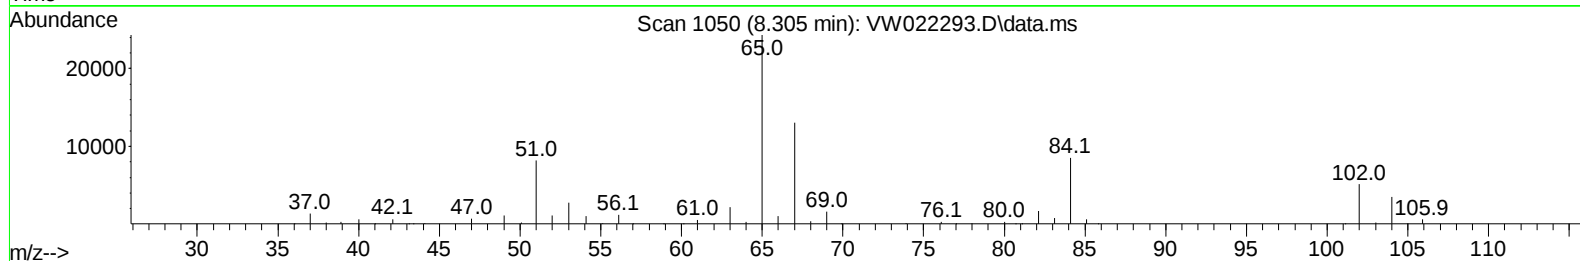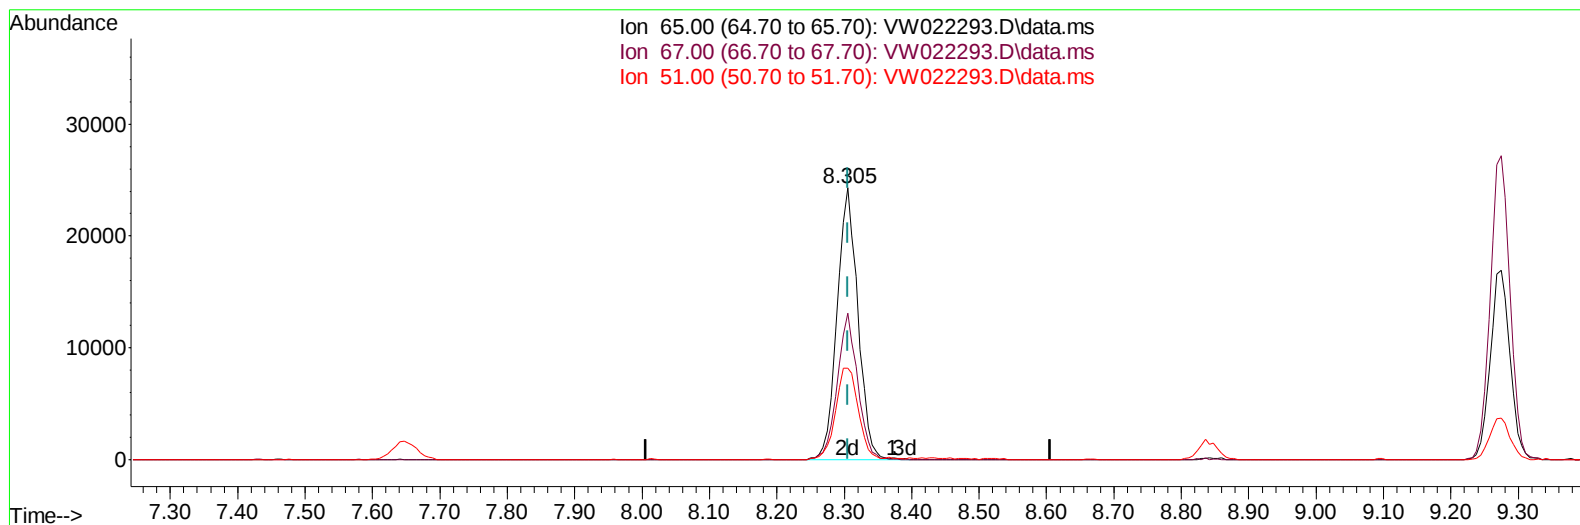

TIC: VW022293.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 24.37 ug/L m

response 51919

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	0.08#
51.00	90.00	0.13#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022293.D
 Acq On : 11 Mar 2022 12:29
 Operator : SY/VA
 Sample : N1819-07
 Misc : 4.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX7

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:03:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		183721	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		169585	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		81963	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		63434	26.472	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	105.880%	
7) Chloroethane-d5	2.879	69		46911	24.881	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	99.520%	
11) 1,1-Dichloroethene-d2	4.013	63		65000	17.713	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	70.840%	
21) 2-Butanone-d5	7.080	46		21829	54.180	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	108.360%	
24) Chloroform-d	7.647	84		100821	24.596	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4	8.305	65		51919m	24.367	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	97.480%	
32) Benzene-d6	8.275	84		195753	24.802	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	99.200%	
36) 1,2-Dichloropropane-d6	9.274	67		55134	25.154	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	100.600%	
41) Toluene-d8	10.323	98		188018	23.962	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	95.840%	
43) trans-1,3-Dichloroprop...	10.579	79		22933	23.598	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	94.400%	
47) 2-Hexanone-d5	10.920	63		17481	48.492	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	96.980%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		47306	24.593	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	98.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152		70333	26.716	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	106.880%	
Target Compounds							Qvalue
13) Acetone	4.123	43		2095m	6.366	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022293.D
Acq On : 11 Mar 2022 12:29
Operator : SY/VA
Sample : N1819-07
Misc : 4.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRX7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:03:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

