




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022296.D
Acq On : 11 Mar 2022 13:41
Operator : SY/VA
Sample : N1819-12
Misc : 7.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRY2

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:04:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

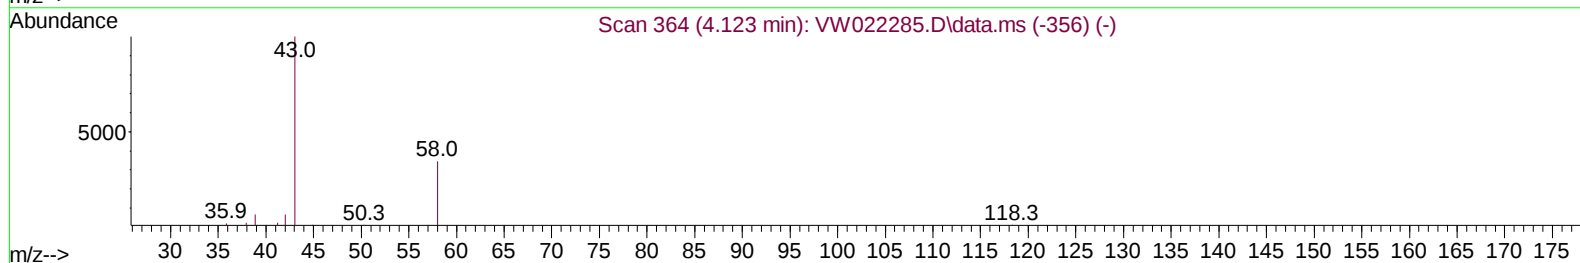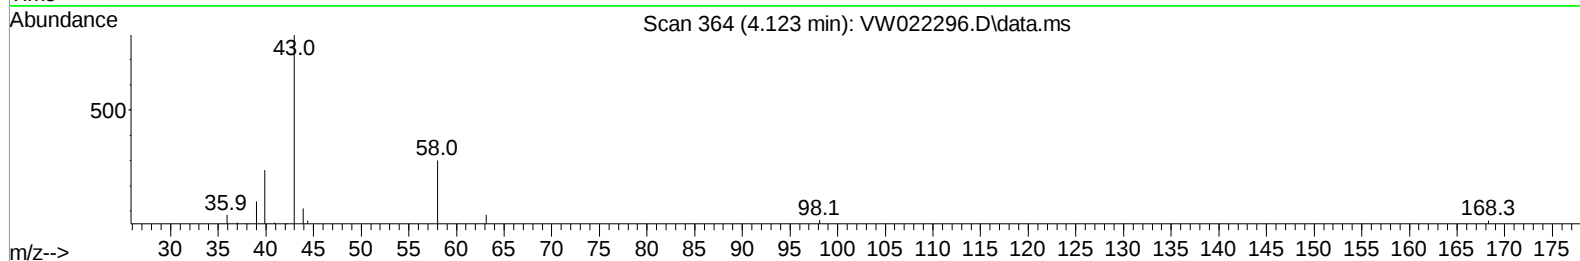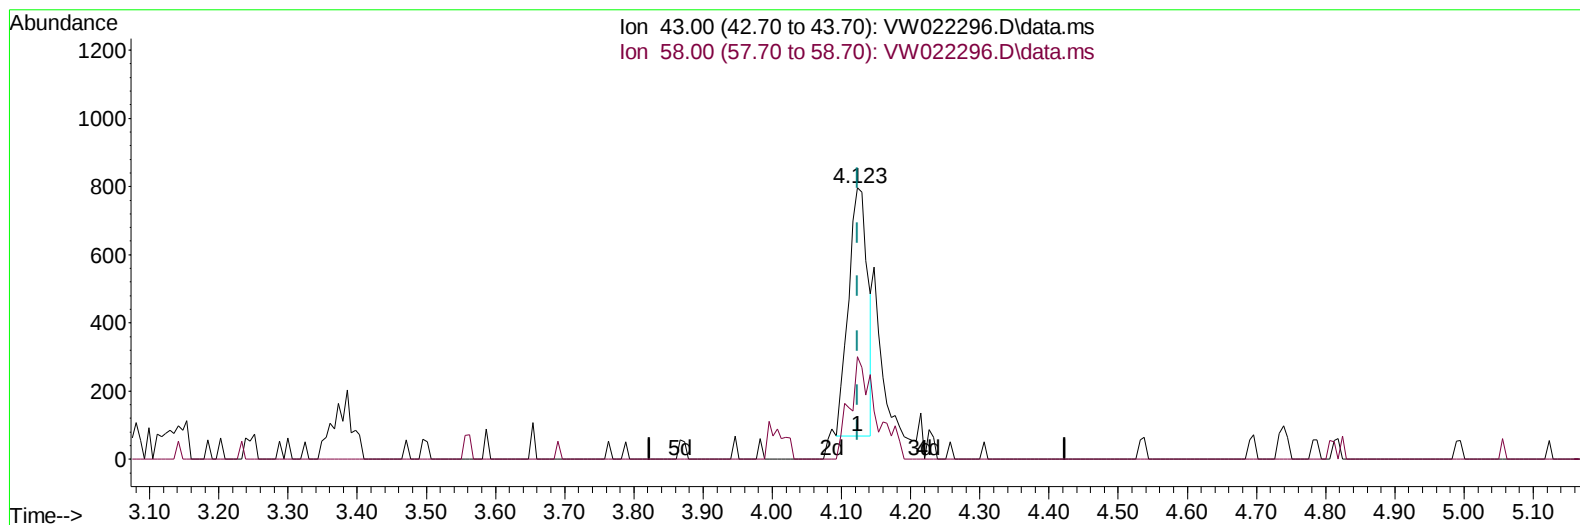

TIC: VW022296.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 4.07 ug/L

response 1395

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	32.26
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022296.D
 Acq On : 11 Mar 2022 13:41
 Operator : SY/VA
 Sample : N1819-12
 Misc : 7.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY2

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:04:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

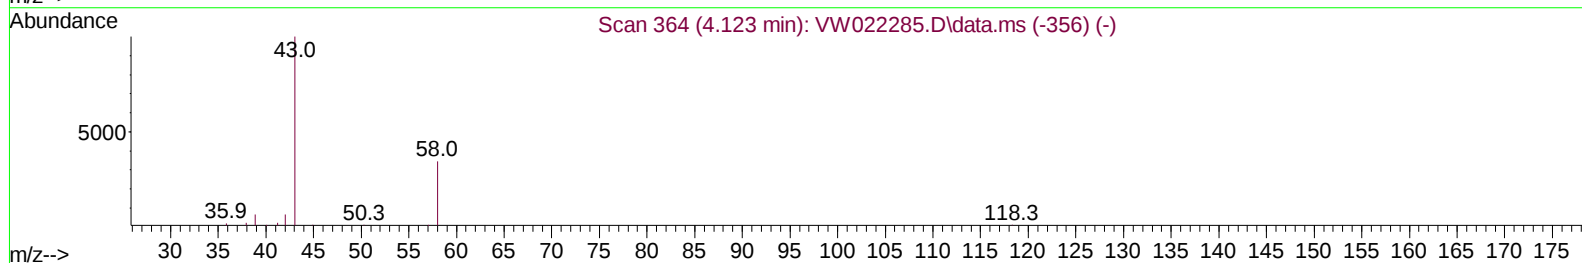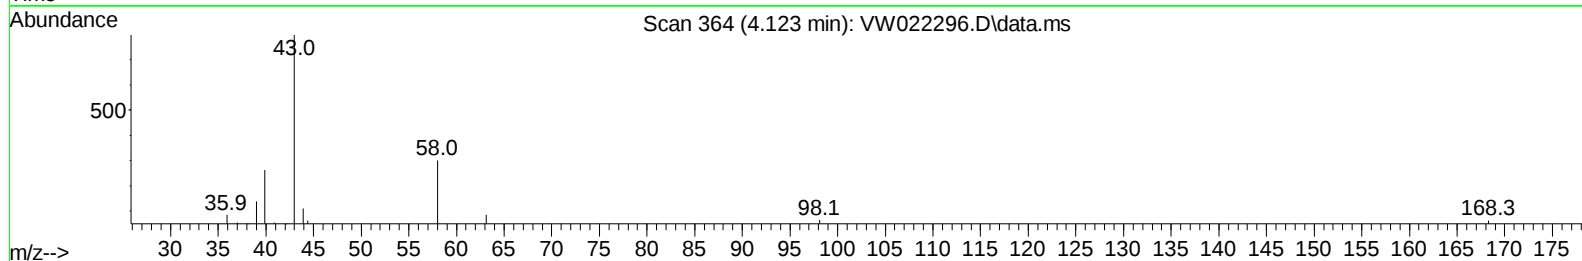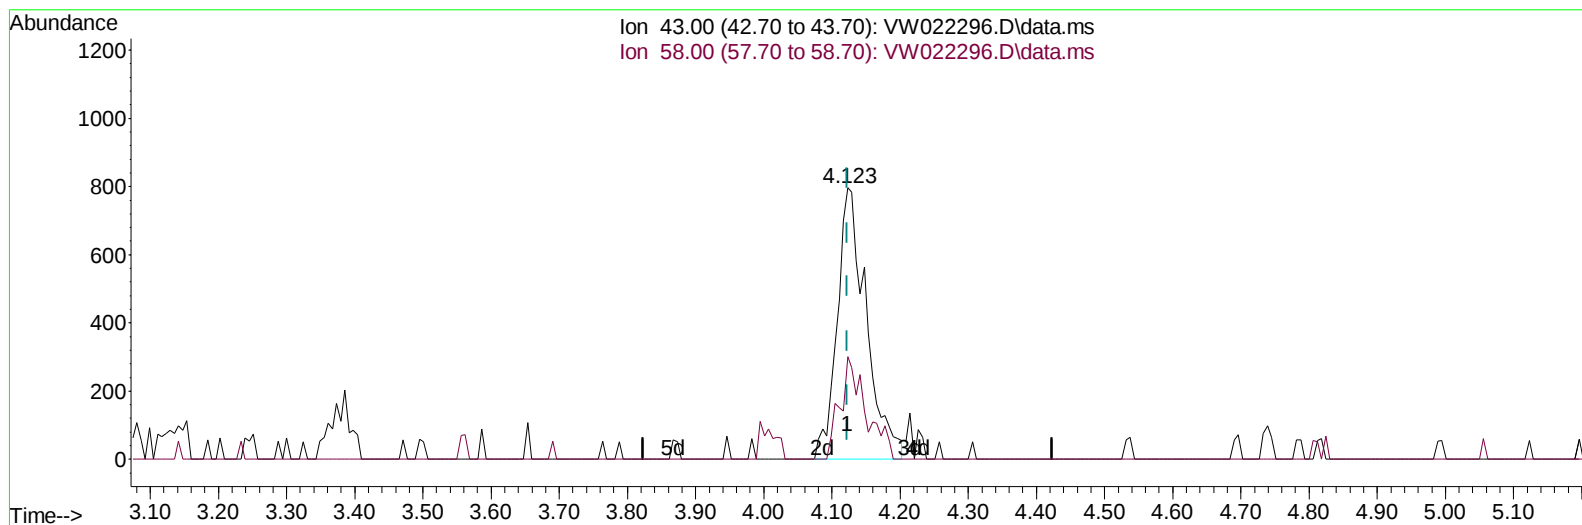

TIC: VW022296.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 6.88 ug/L m

response 2358

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	19.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022296.D
 Acq On : 11 Mar 2022 13:41
 Operator : SY/VA
 Sample : N1819-12
 Misc : 7.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:04:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

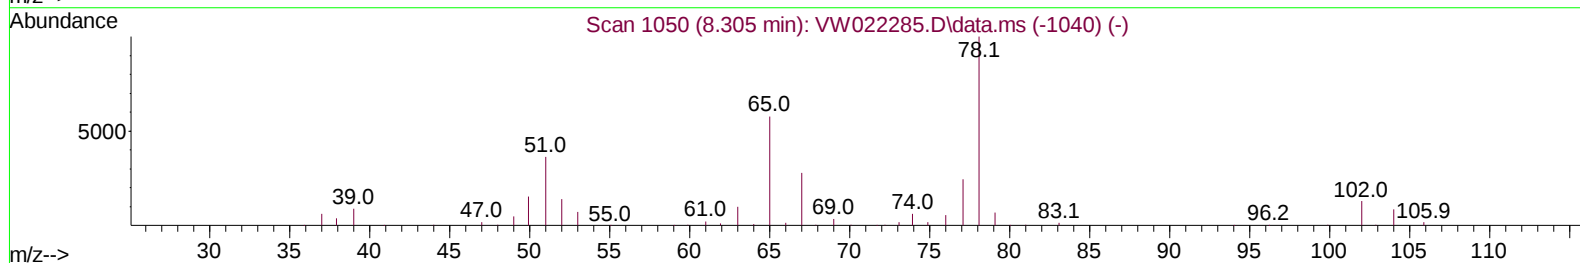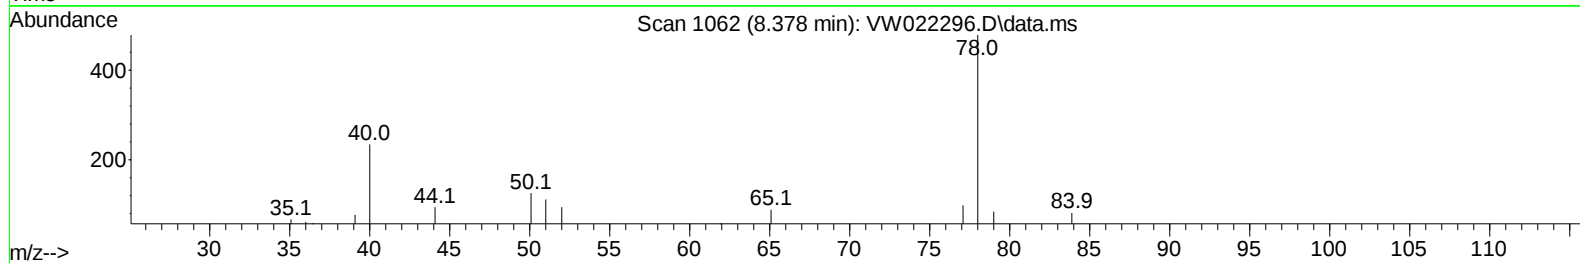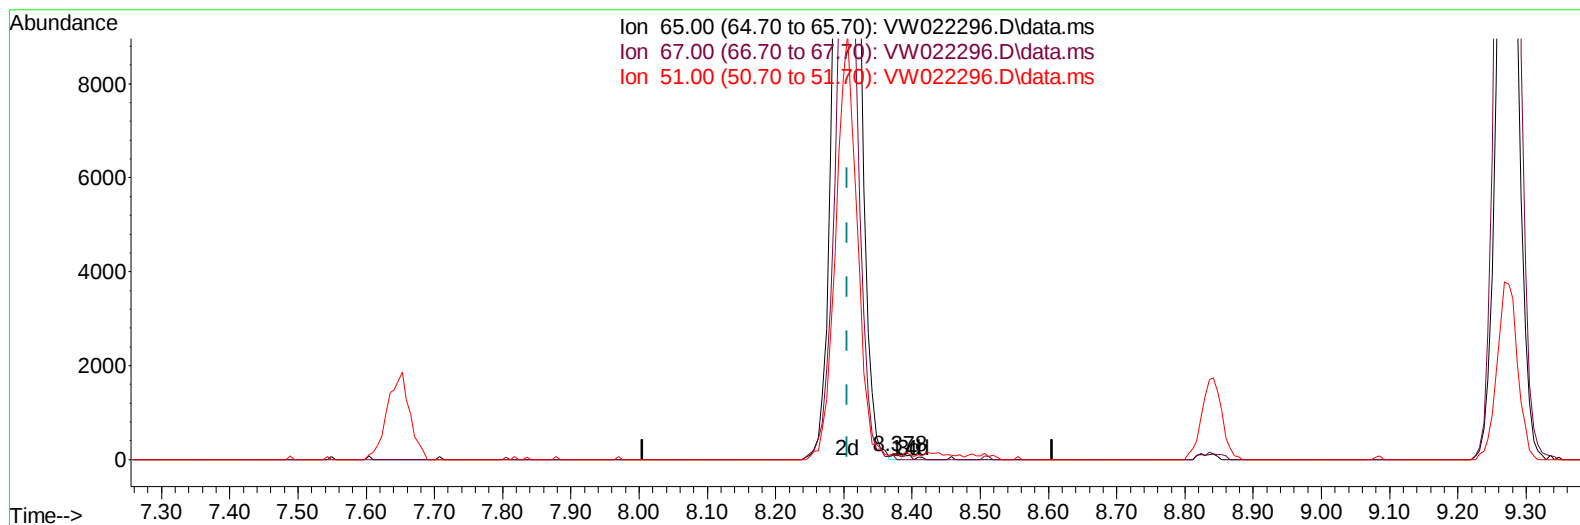

TIC: VW022296.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.378min (+ 0.073) 0.04 ug/L

response 89

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	66.29
51.00	90.00	87.64
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022296.D
 Acq On : 11 Mar 2022 13:41
 Operator : SY/VA
 Sample : N1819-12
 Misc : 7.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY2

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:04:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

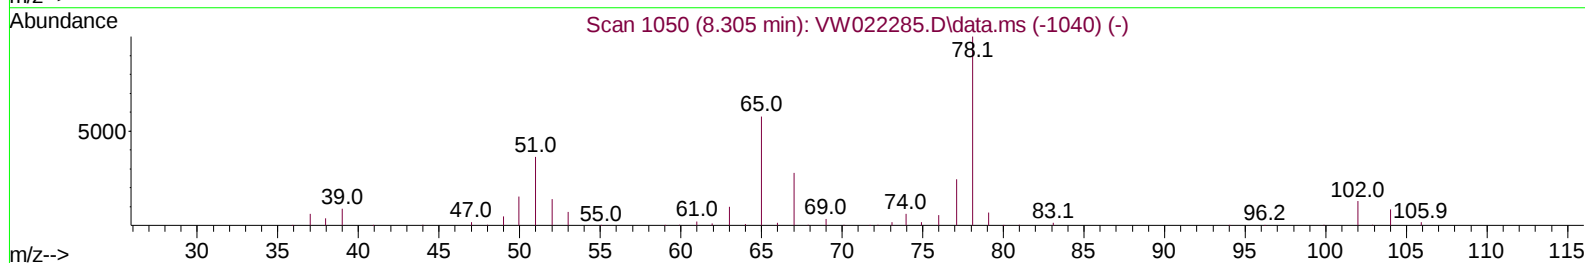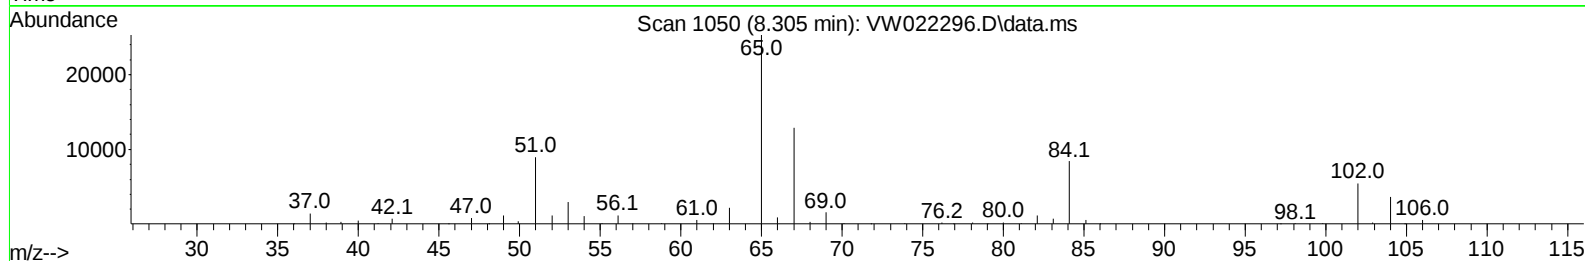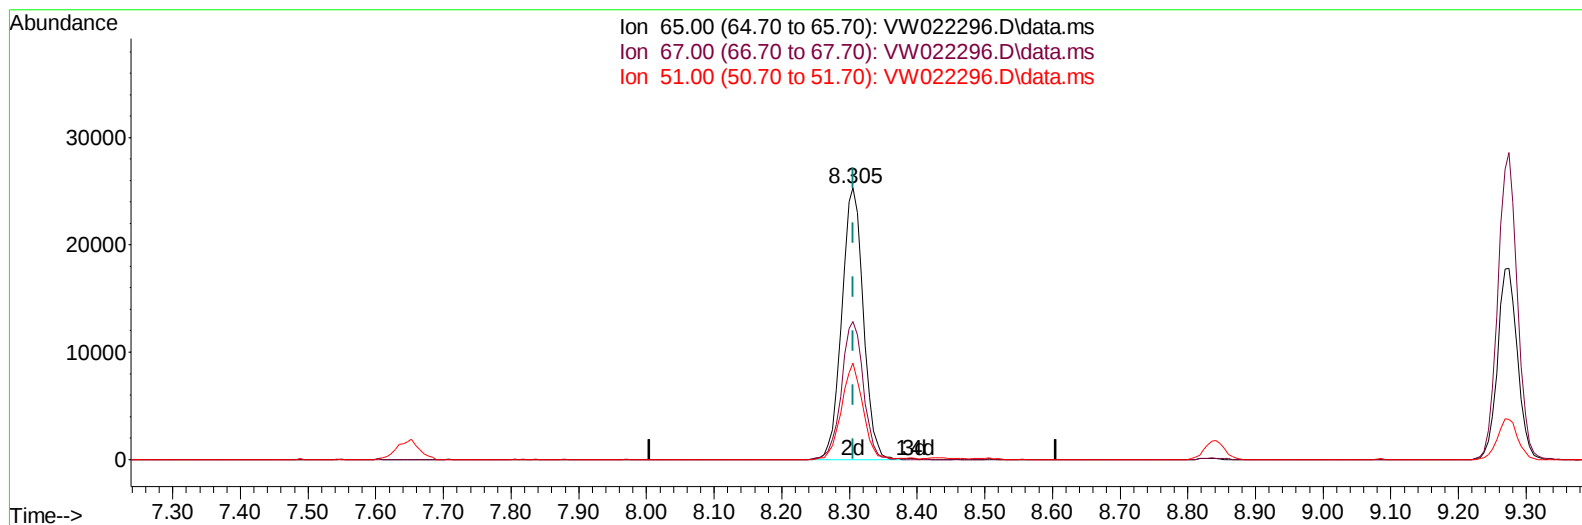

TIC: VW022296.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 25.23 ug/L m

response 55962

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	0.11#
51.00	90.00	0.14#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022296.D
 Acq On : 11 Mar 2022 13:41
 Operator : SY/VA
 Sample : N1819-12
 Misc : 7.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:04:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		191260	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		177640	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		81666	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		66806	26.780	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	107.120%	
7) Chloroethane-d5	2.879	69		49048	24.989	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	99.960%	
11) 1,1-Dichloroethene-d2	4.013	63		63445	16.608	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	66.440%	
21) 2-Butanone-d5	7.074	46		21874	52.151	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	104.300%	
24) Chloroform-d	7.647	84		103560	24.268	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	97.080%	
26) 1,2-Dichloroethane-d4	8.305	65		55962m	25.229	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	100.920%	
32) Benzene-d6	8.275	84		200400	24.240	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	96.960%	
36) 1,2-Dichloropropane-d6	9.275	67		57255	24.938	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	99.760%	
41) Toluene-d8	10.323	98		193050	23.488	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	93.960%	
43) trans-1,3-Dichloroprop...	10.573	79		23639	23.221	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	92.880%	
47) 2-Hexanone-d5	10.921	63		18223	48.258	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	96.520%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		48934	24.286	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	97.160%	
66) 1,2-Dichlorobenzene-d4	13.853	152		70277	26.792	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	107.160%	
Target Compounds							
13) Acetone	4.123	43		2358m	6.883	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022296.D
Acq On : 11 Mar 2022 13:41
Operator : SY/VA
Sample : N1819-12
Misc : 7.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:04:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

