




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022300.D
 Acq On : 11 Mar 2022 15:18
 Operator : SY/VA
 Sample : N1819-11
 Misc : 5.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY1

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:04:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

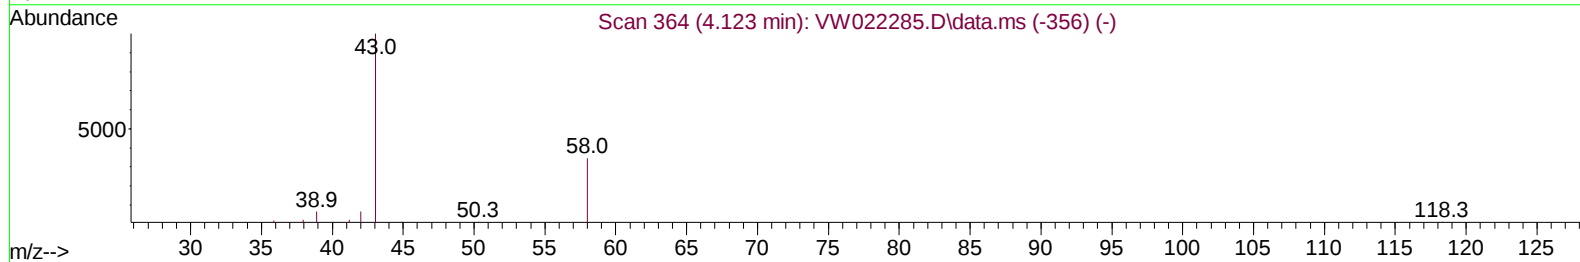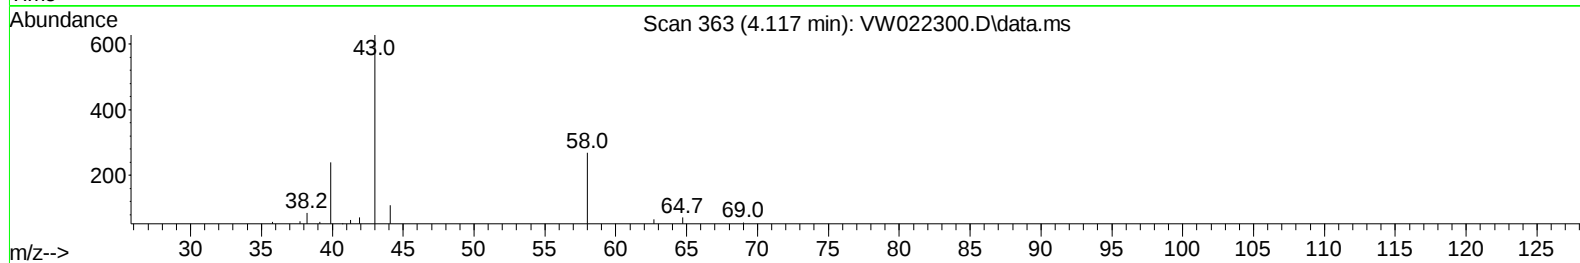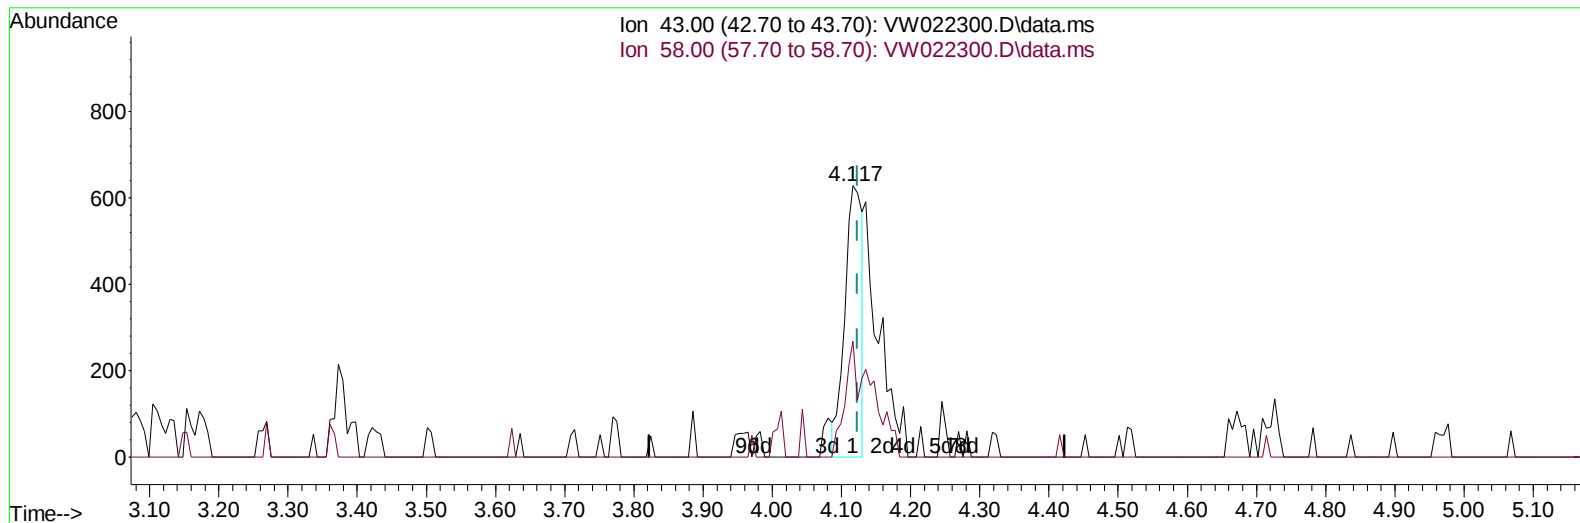

TIC: VW022300.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 3.25 ug/L

response 1082

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	29.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022300.D
 Acq On : 11 Mar 2022 15:18
 Operator : SY/VA
 Sample : N1819-11
 Misc : 5.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY1

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:04:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

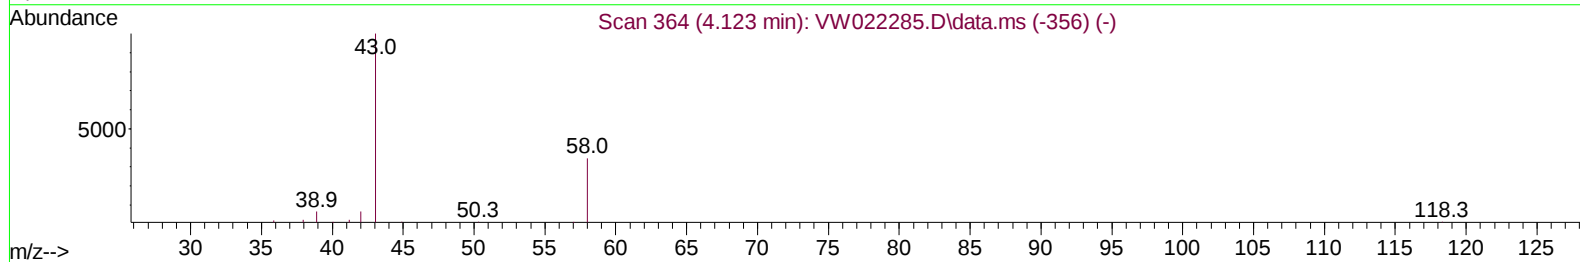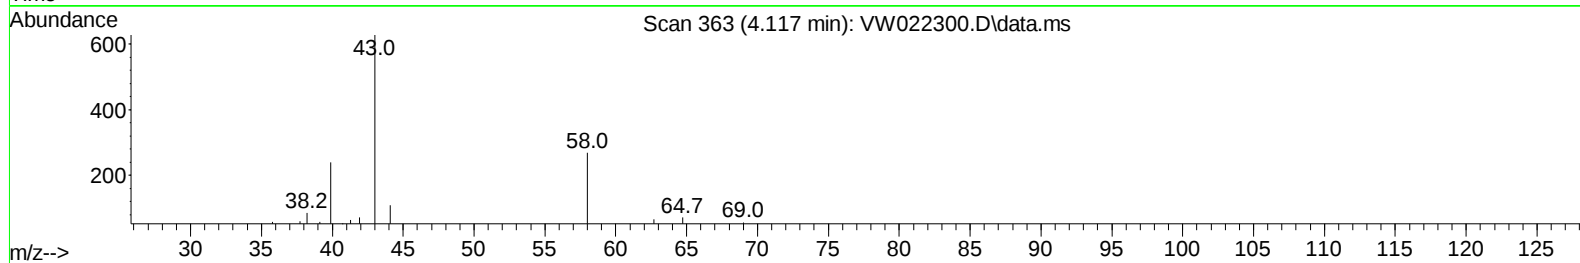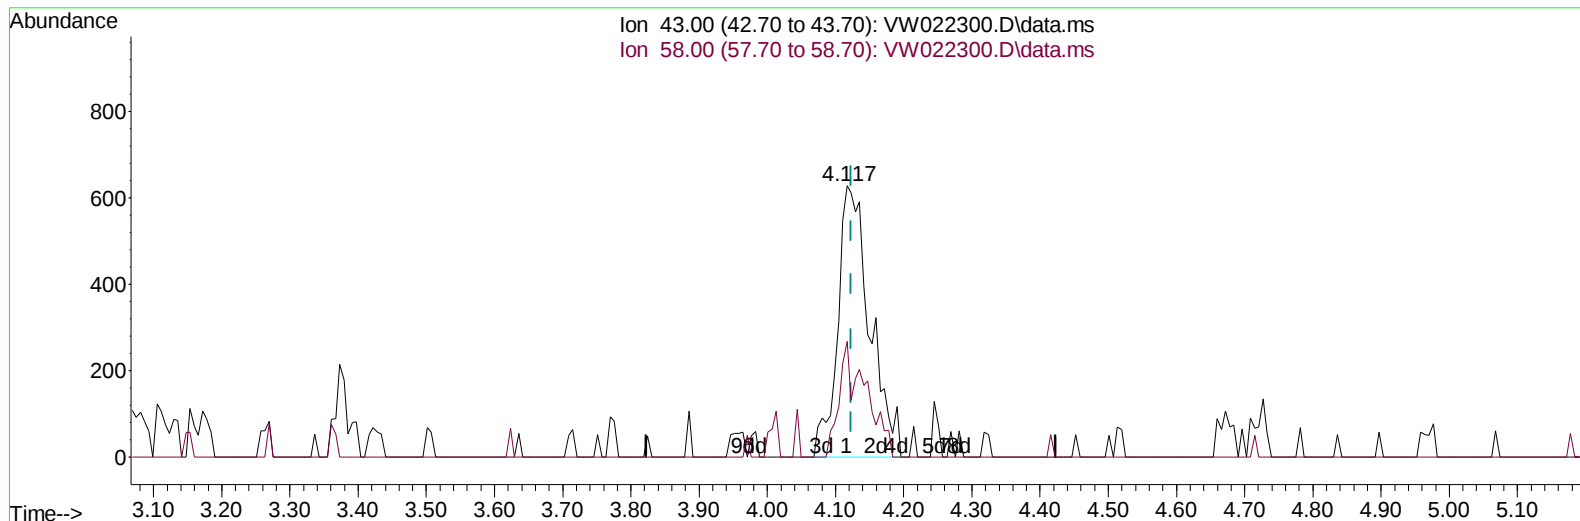

TIC: VW022300.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 6.18 ug/L m

response 2059

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	15.54
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022300.D
 Acq On : 11 Mar 2022 15:18
 Operator : SY/VA
 Sample : N1819-11
 Misc : 5.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:04:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	185878	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	170302	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81568	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	67441	27.817	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	111.280%	
7) Chloroethane-d5	2.873	69	53077	27.825	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	111.280%	
11) 1,1-Dichloroethene-d2	4.013	63	62774	16.908	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	67.640%	
21) 2-Butanone-d5	7.074	46	27171	66.656	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	133.320%	
24) Chloroform-d	7.647	84	101701	24.523	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.080%	
26) 1,2-Dichloroethane-d4	8.305	65	55546	25.766	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.080%	
32) Benzene-d6	8.275	84	197301	24.893	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	99.560%	
36) 1,2-Dichloropropane-d6	9.275	67	56279	25.569	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.280%	
41) Toluene-d8	10.323	98	189893	24.099	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	10.579	79	23623	24.205	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	96.840%	
47) 2-Hexanone-d5	10.921	63	21835	60.315	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.620%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	54424	28.174	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	112.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	70165	26.782	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	107.120%	
Target Compounds						
13) Acetone	4.117	43	2059m	6.184	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022300.D
Acq On : 11 Mar 2022 15:18
Operator : SY/VA
Sample : N1819-11
Misc : 5.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRY1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:04:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

