




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022303.D
 Acq On : 11 Mar 2022 16:31
 Operator : SY/VA
 Sample : N1819-18
 Misc : 5.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY8

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:05:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

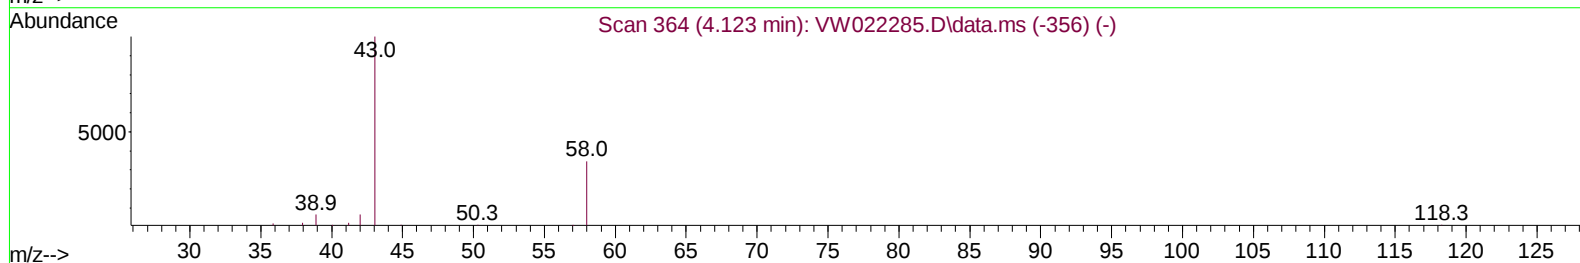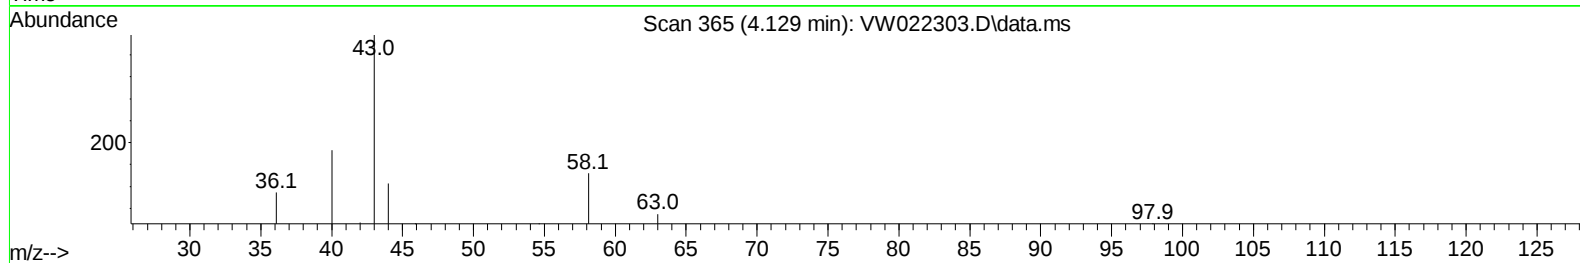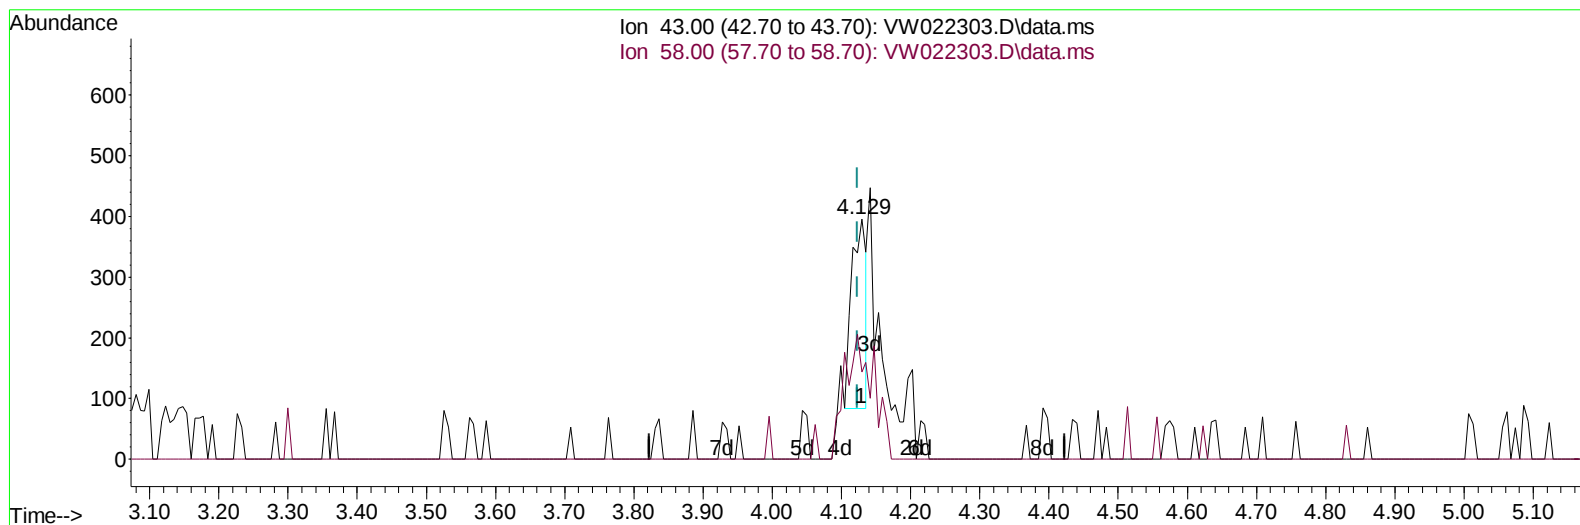

TIC: VW022303.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 1.82 ug/L

response 455

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	61.76
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022303.D
 Acq On : 11 Mar 2022 16:31
 Operator : SY/VA
 Sample : N1819-18
 Misc : 5.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY8

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:05:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

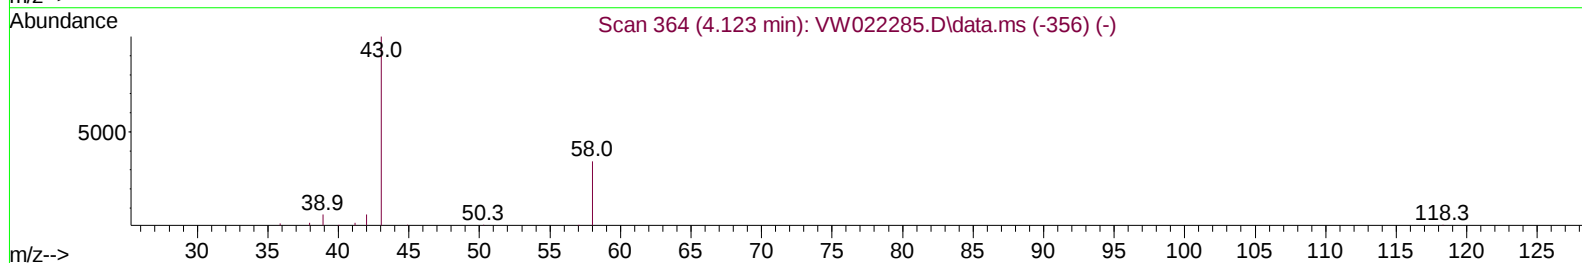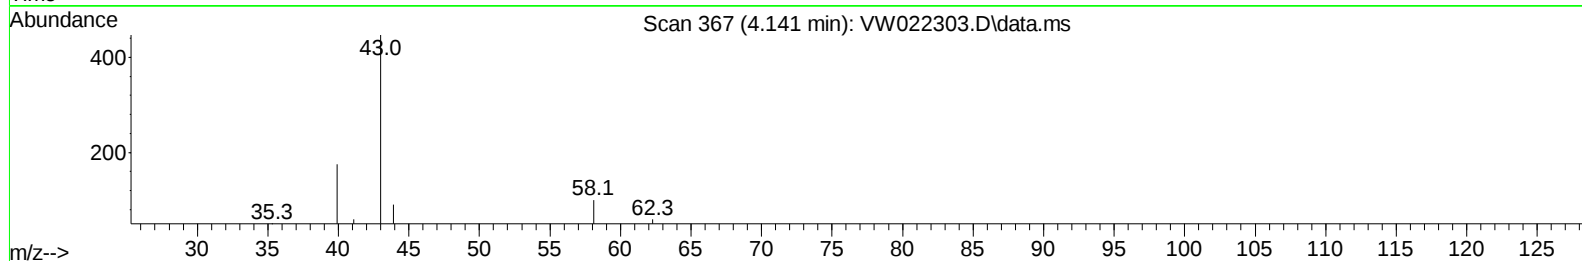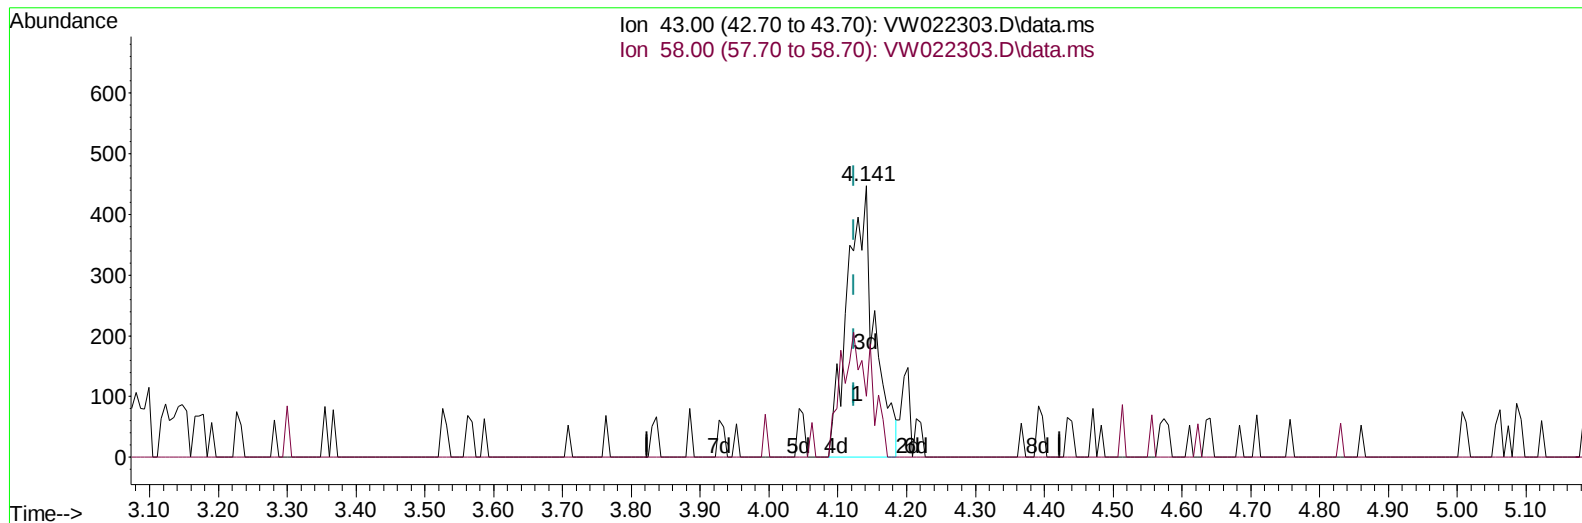

TIC: VW022303.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 4.89 ug/L m

response 1224

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	22.96
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022303.D
 Acq On : 11 Mar 2022 16:31
 Operator : SY/VA
 Sample : N1819-18
 Misc : 5.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY8

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:05:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	139650	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	131182	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	63601	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	50457	27.701	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	110.800%	
7) Chloroethane-d5	2.879	69	39811	27.779	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	111.120%	
11) 1,1-Dichloroethene-d2	4.013	63	46075	16.518	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	66.080%	
21) 2-Butanone-d5	7.074	46	20115	65.681	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	131.360%	
24) Chloroform-d	7.647	84	80062	25.696	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	102.800%	
26) 1,2-Dichloroethane-d4	8.305	65	44657	27.573	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	110.280%	
32) Benzene-d6	8.275	84	151863	24.874	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	99.480%	
36) 1,2-Dichloropropane-d6	9.274	67	44202	26.071	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	104.280%	
41) Toluene-d8	10.323	98	140631	23.169	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	92.680%	
43) trans-1,3-Dichloroprop...	10.573	79	18987	25.257	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	101.040%	
47) 2-Hexanone-d5	10.921	63	16539	59.310	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	118.620%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	43737	29.394	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	117.560%	
66) 1,2-Dichlorobenzene-d4	13.847	152	55534	27.185	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	108.760%	
Target Compounds						
13) Acetone	4.141	43	1224m	4.893	ug/L	
20) cis-1,2-Dichloroethene	7.171	96	5673	3.305	ug/L	90
46) Tetrachloroethene	10.866	164	1600	1.006	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022303.D
Acq On : 11 Mar 2022 16:31
Operator : SY/VA
Sample : N1819-18
Misc : 5.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRY8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:05:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

