




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022304.D
Acq On : 11 Mar 2022 16:55
Operator : SY/VA
Sample : N1819-19
Misc : 5.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRY9

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:05:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

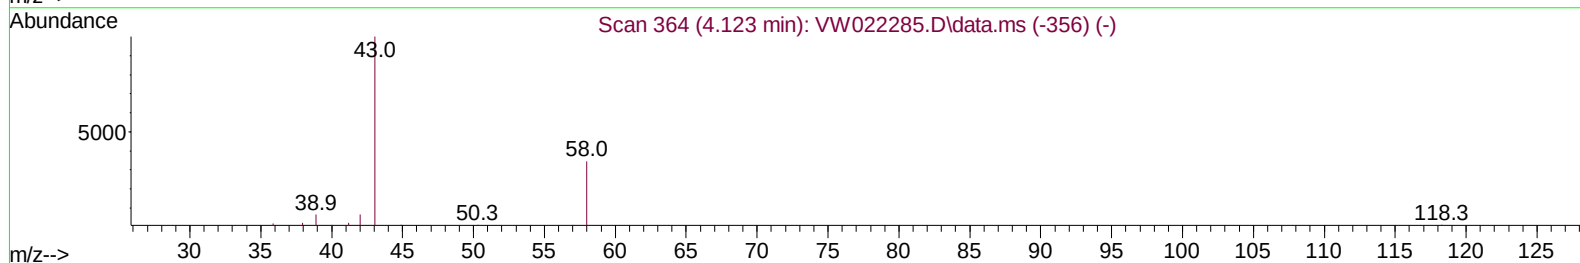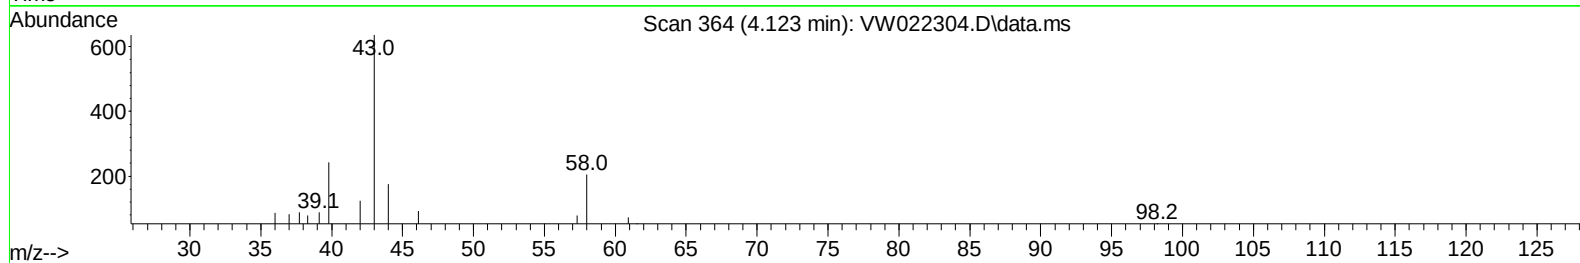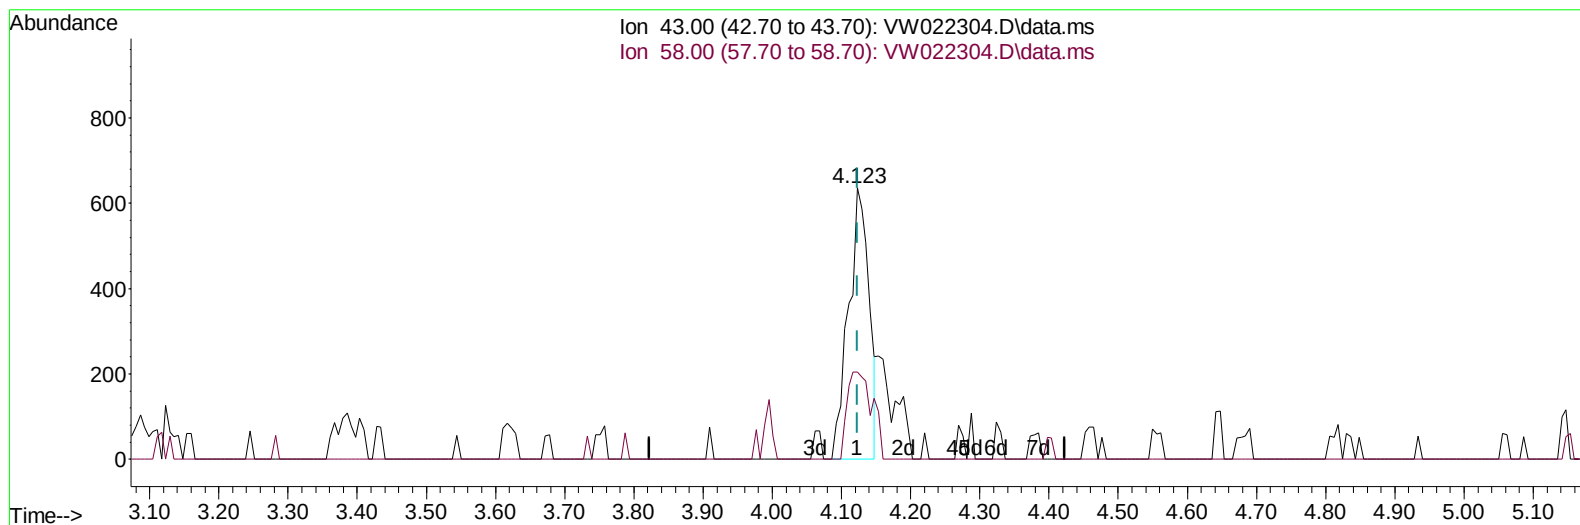

TIC: VW022304.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 4.11 ug/L

response 1311

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	32.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022304.D
 Acq On : 11 Mar 2022 16:55
 Operator : SY/VA
 Sample : N1819-19
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY9

Manual IntegrationsAPPROVED

Quant Time: Mar 11 21:05:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

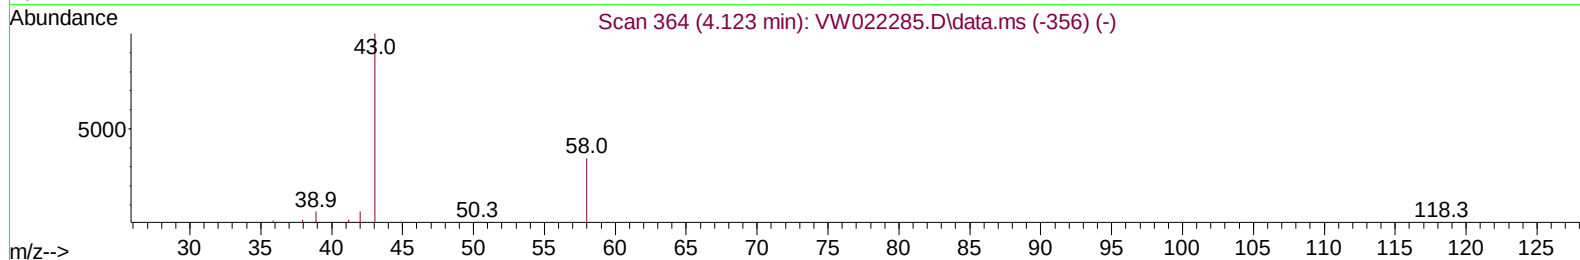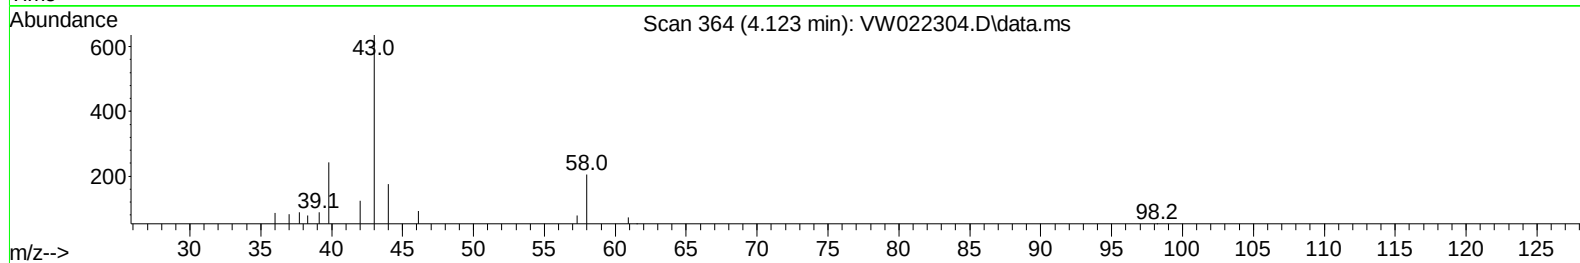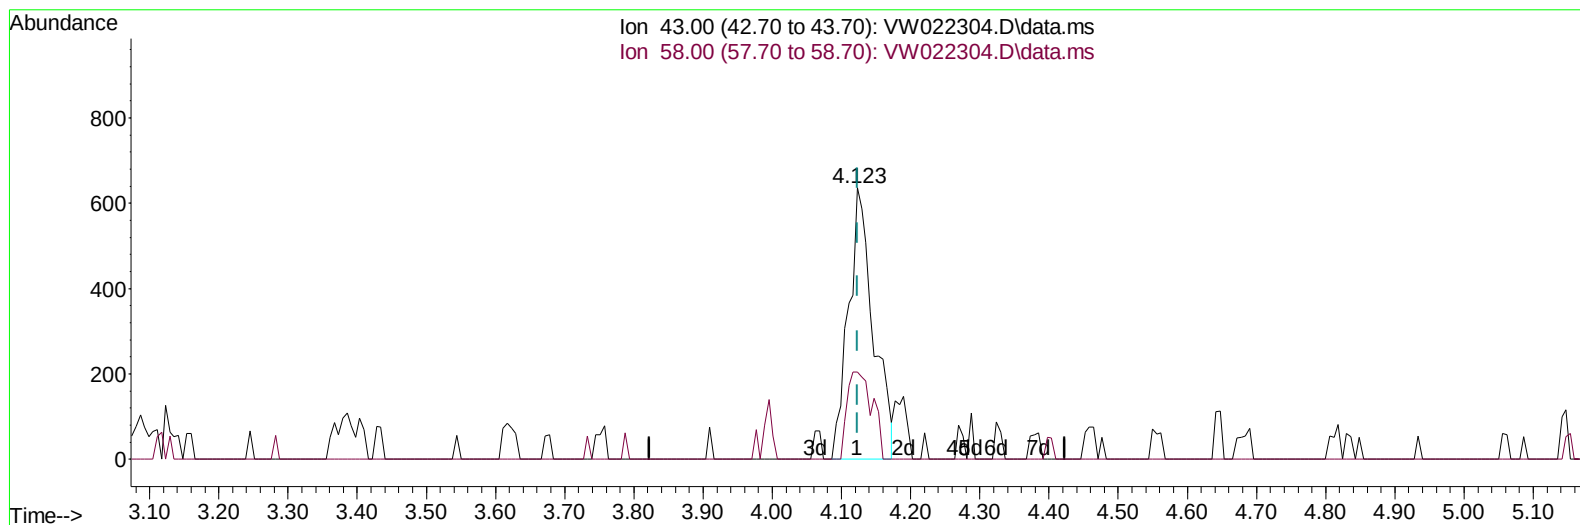

TIC: VW022304.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 4.95 ug/L m

response 1579

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	26.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022304.D
 Acq On : 11 Mar 2022 16:55
 Operator : SY/VA
 Sample : N1819-19
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:05:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	178143	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	166652	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80998	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	59062	25.419	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	101.680%	
7) Chloroethane-d5	2.879	69	46671	25.529	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	102.120%	
11) 1,1-Dichloroethene-d2	4.007	63	54907	15.431	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	61.720%	
21) 2-Butanone-d5	7.068	46	21488	55.003	ug/L	-0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	110.000%	
24) Chloroform-d	7.647	84	89683	22.564	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	90.240%	
26) 1,2-Dichloroethane-d4	8.305	65	48409	23.431	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	93.720%	
32) Benzene-d6	8.275	84	173025	22.309	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	89.240%	
36) 1,2-Dichloropropane-d6	9.274	67	49430	22.949	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	91.800%	
41) Toluene-d8	10.323	98	163316	21.180	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	84.720%	
43) trans-1,3-Dichloroprop...	10.573	79	20527	21.494	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	85.960%	
47) 2-Hexanone-d5	10.921	63	17434	49.213	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.420%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	45988	24.328	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	97.320%	
66) 1,2-Dichlorobenzene-d4	13.847	152	60375	23.207	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.840%	
Target Compounds						
13) Acetone	4.123	43	1579m	4.949	ug/L	
20) cis-1,2-Dichloroethene	7.177	96	1596	0.729	ug/L	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022304.D
Acq On : 11 Mar 2022 16:55
Operator : SY/VA
Sample : N1819-19
Misc : 5.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:05:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

