

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022290.D
 Acq On : 11 Mar 2022 11:16
 Operator : SY/VA
 Sample : N1819-04
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX6

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/13/2022
 Supervised By : Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:02:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	185750	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	167916	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80443	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	67581	27.894	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 111.560%			
7) Chloroethane-d5	2.879	69	44740	23.470	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 93.880%			
11) 1,1-Dichloroethene-d2	4.013	63	66972	18.051	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 72.200%			
21) 2-Butanone-d5	7.074	46	17924	44.001	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 88.000%			
24) Chloroform-d	7.647	84	103891	25.068	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 100.280%			
26) 1,2-Dichloroethane-d4	8.305	65	51199	23.766	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 95.080%			
32) Benzene-d6	8.275	84	203496	26.040	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 104.160%			
36) 1,2-Dichloropropane-d6	9.275	67	55709	25.669	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 102.680%			
41) Toluene-d8	10.323	98	196452	25.286	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 101.160%			
43) trans-1,3-Dichloroprop...	10.573	79	21529	22.373	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 89.480%			
47) 2-Hexanone-d5	10.921	63	14267	39.970	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 79.940%			
56) 1,1,2,2-Tetrachloroeth...	12.689	84	41863	21.979	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 87.920%			
66) 1,2-Dichlorobenzene-d4	13.853	152	65787	25.462	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 101.840%			
Target Compounds					Qvalue	
13) Acetone	4.123	43	1498m	4.503	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022290.D
Acq On : 11 Mar 2022 11:16
Operator : SY/VA
Sample : N1819-04
Misc : 5.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBRX6

Quant Time: Mar 11 21:02:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

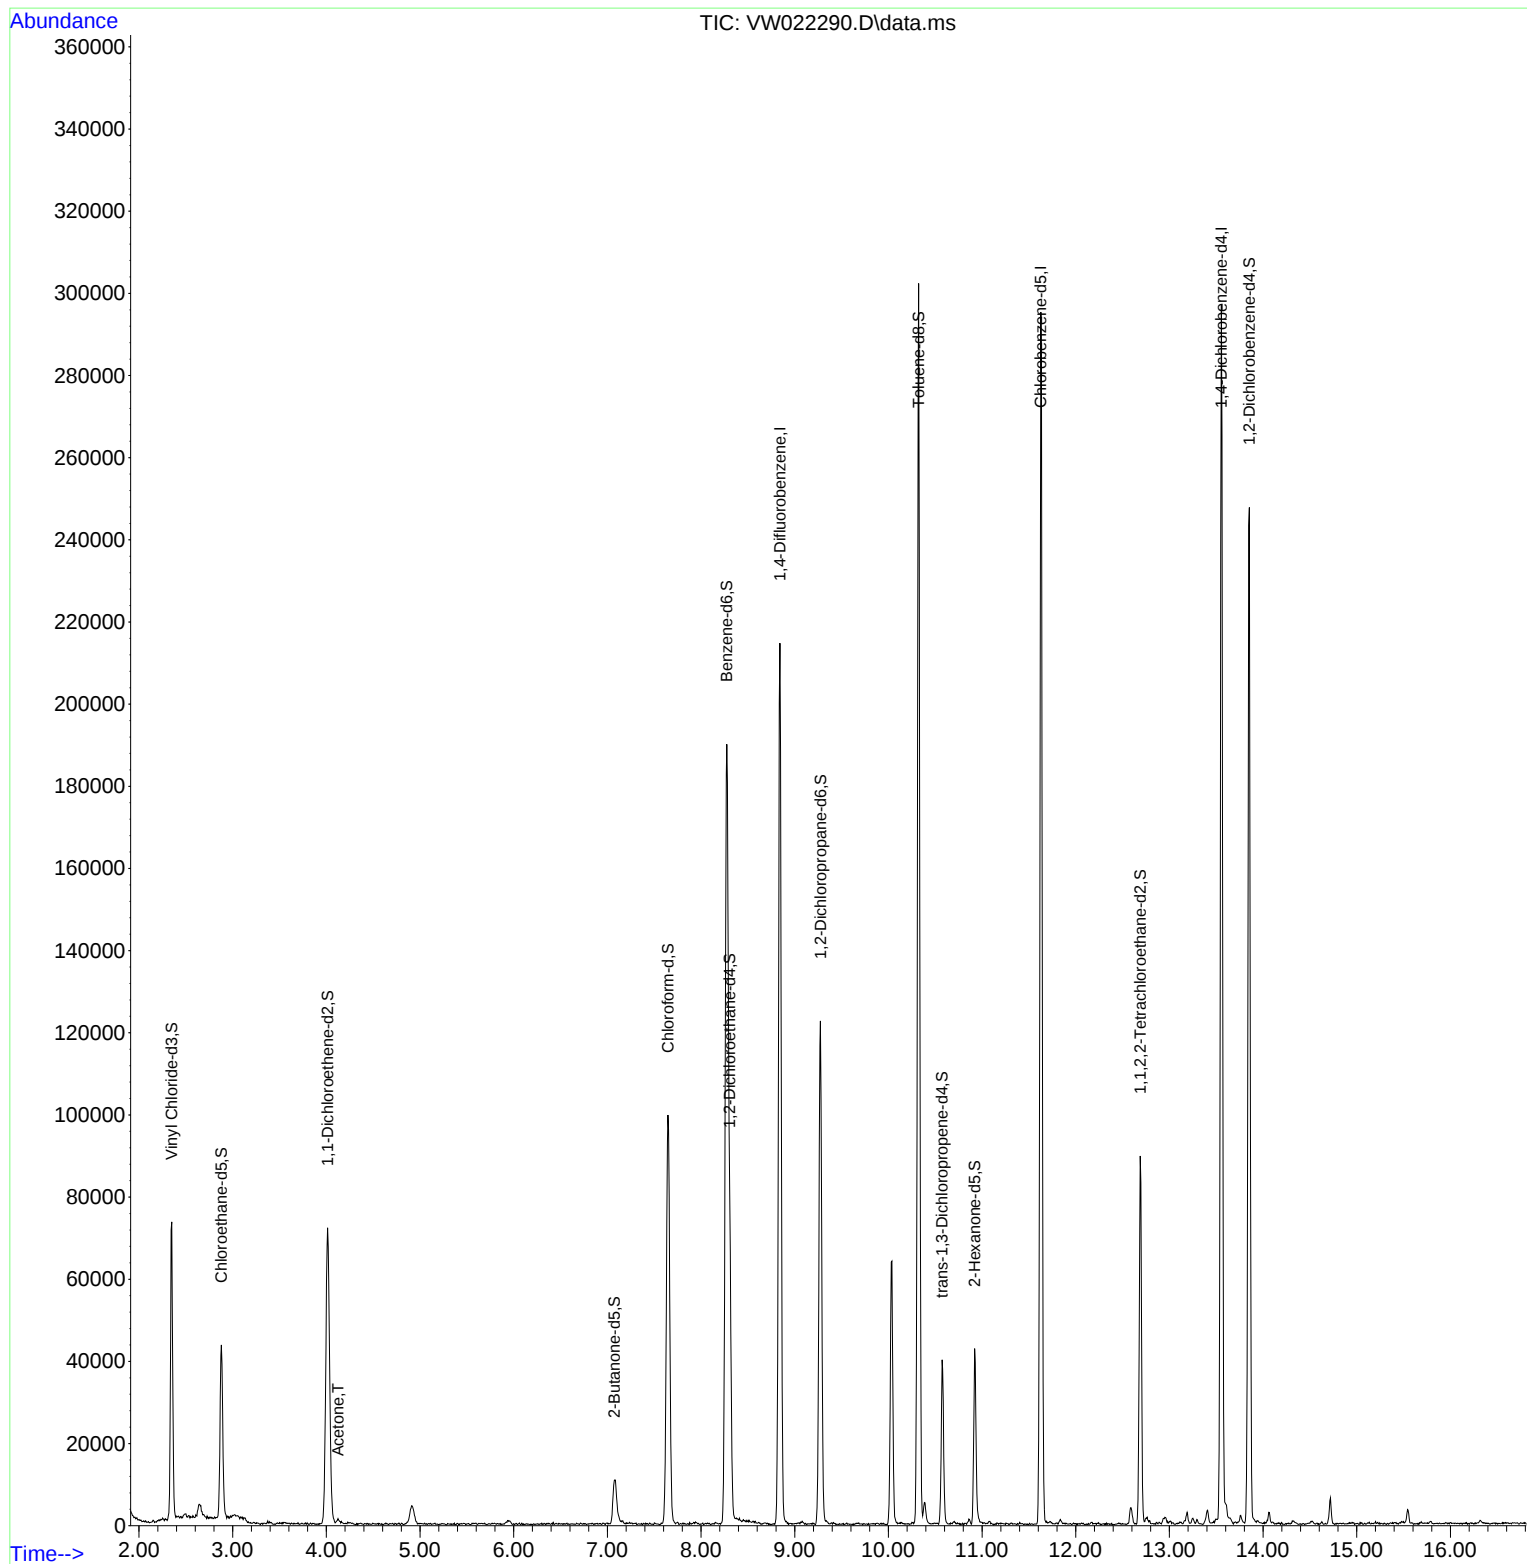

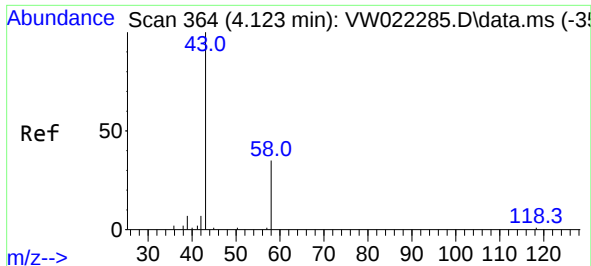

#13
 Acetone
 Concen: 4.503 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW022290.D
 Acq: 11 Mar 2022 11:16

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRX6

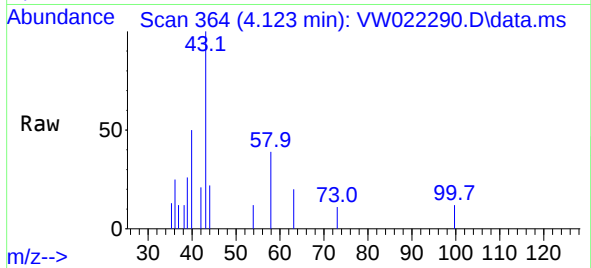

Tgt Ion: 43 Resp: 1498
 Ion Ratio Lower Upper
 43 100
 58 18.0 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

