

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022296.D
 Acq On : 11 Mar 2022 13:41
 Operator : SY/VA
 Sample : N1819-12
 Misc : 7.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 21:04:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	191260	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	177640	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81666	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	66806	26.780	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 107.120%			
7) Chloroethane-d5	2.879	69	49048	24.989	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 99.960%			
11) 1,1-Dichloroethene-d2	4.013	63	63445	16.608	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 66.440%			
21) 2-Butanone-d5	7.074	46	21874	52.151	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 104.300%			
24) Chloroform-d	7.647	84	103560	24.268	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 97.080%			
26) 1,2-Dichloroethane-d4	8.305	65	55962m	25.229	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 100.920%			
32) Benzene-d6	8.275	84	200400	24.240	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 96.960%			
36) 1,2-Dichloropropane-d6	9.275	67	57255	24.938	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 99.760%			
41) Toluene-d8	10.323	98	193050	23.488	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 93.960%			
43) trans-1,3-Dichloroprop...	10.573	79	23639	23.221	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 92.880%			
47) 2-Hexanone-d5	10.921	63	18223	48.258	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 96.520%			
56) 1,1,2,2-Tetrachloroeth...	12.689	84	48934	24.286	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 97.160%			
66) 1,2-Dichlorobenzene-d4	13.853	152	70277	26.792	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 107.160%			
Target Compounds					Qvalue	
13) Acetone	4.123	43	2358m	6.883	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022296.D
Acq On : 11 Mar 2022 13:41
Operator : SY/VA
Sample : N1819-12
Misc : 7.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBRY2

Quant Time: Mar 11 21:04:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

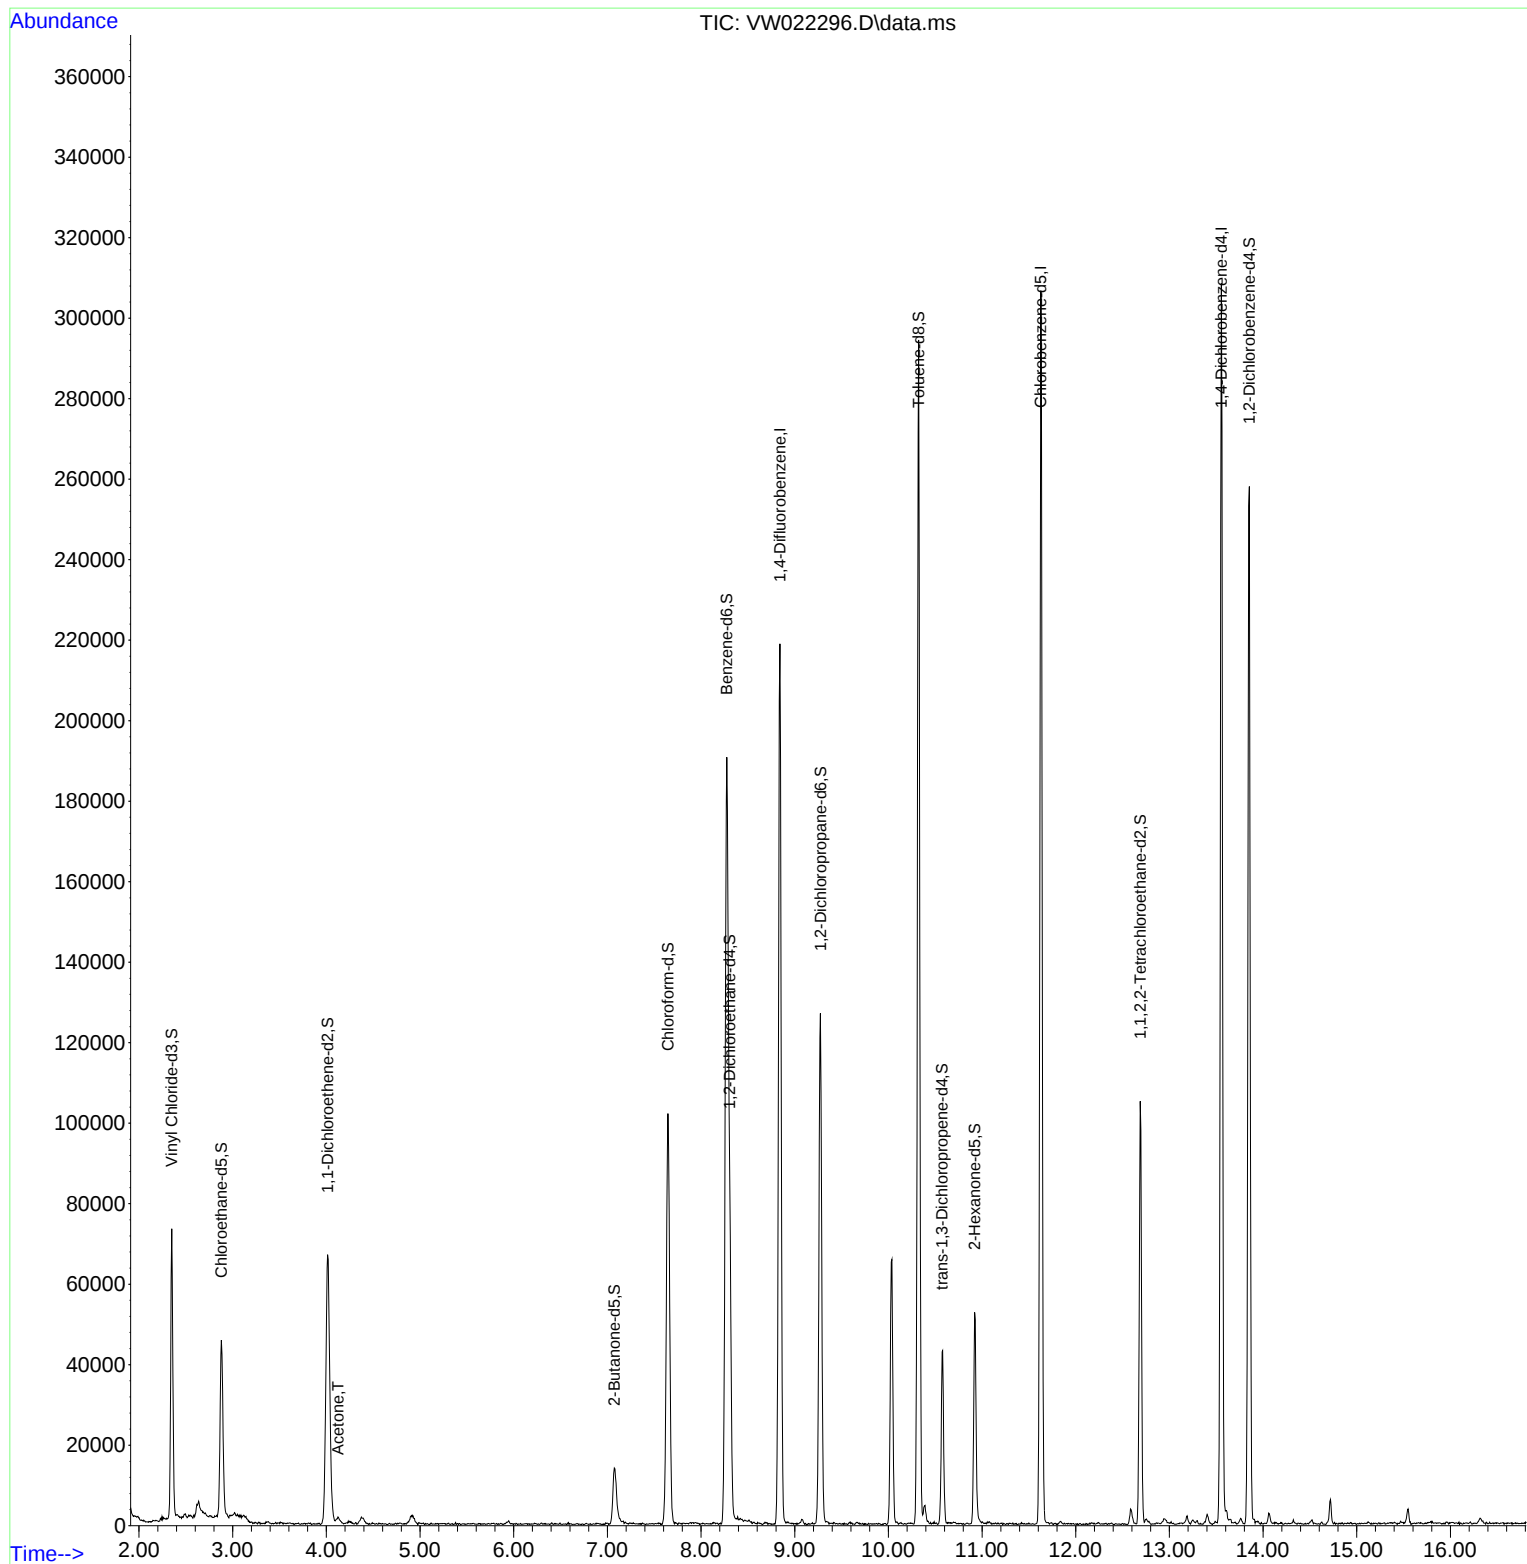

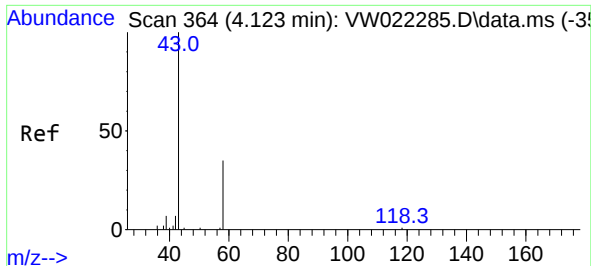

#13

Acetone

Concen: 6.883 ug/L m

RT: 4.123 min Scan# 30

Delta R.T. 0.000 min

Lab File: VW022296.D

Acq: 11 Mar 2022 13:41

Instrument :

MSVOA_W

ClientSampleId :

DBRY2

Tgt Ion: 43 Resp: 235

Ion Ratio Lower Upper

43 100

58 19.1 0.0 69.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022

Supervised By :Mahesh Dadoda 03/14/2022

