

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022301.D
 Acq On : 11 Mar 2022 15:42
 Operator : SY/VA
 Sample : N1819-13
 Misc : 7.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRY3

Quant Time: Mar 11 21:05:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.836	114	173907	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	162279	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81428	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	55947	24.665	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.640%
7) Chloroethane-d5	2.873	69	42341	23.724	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.880%
11) 1,1-Dichloroethene-d2	4.013	63	51654	14.870	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.480%
21) 2-Butanone-d5	7.074	46	27698	72.626	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	145.260%#
24) Chloroform-d	7.647	84	86562	22.309	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.240%
26) 1,2-Dichloroethane-d4	8.305	65	50680	25.127	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.520%
32) Benzene-d6	8.275	84	169319	22.419	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.680%
36) 1,2-Dichloropropane-d6	9.268	67	49145	23.431	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.720%
41) Toluene-d8	10.323	98	156407	20.831	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.320%
43) trans-1,3-Dichloroprop...	10.573	79	21986	23.642	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.560%
47) 2-Hexanone-d5	10.921	63	23037	66.781	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	133.560%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	52872	28.724	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	63249	24.183	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.720%
Target Compounds					Qvalue	
13) Acetone	4.123	43	4219	13.545	ug/L	99
14) Carbon disulfide	4.373	76	6621	1.422	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022301.D
Acq On : 11 Mar 2022 15:42
Operator : SY/VA
Sample : N1819-13
Misc : 7.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRY3

Quant Time: Mar 11 21:05:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration




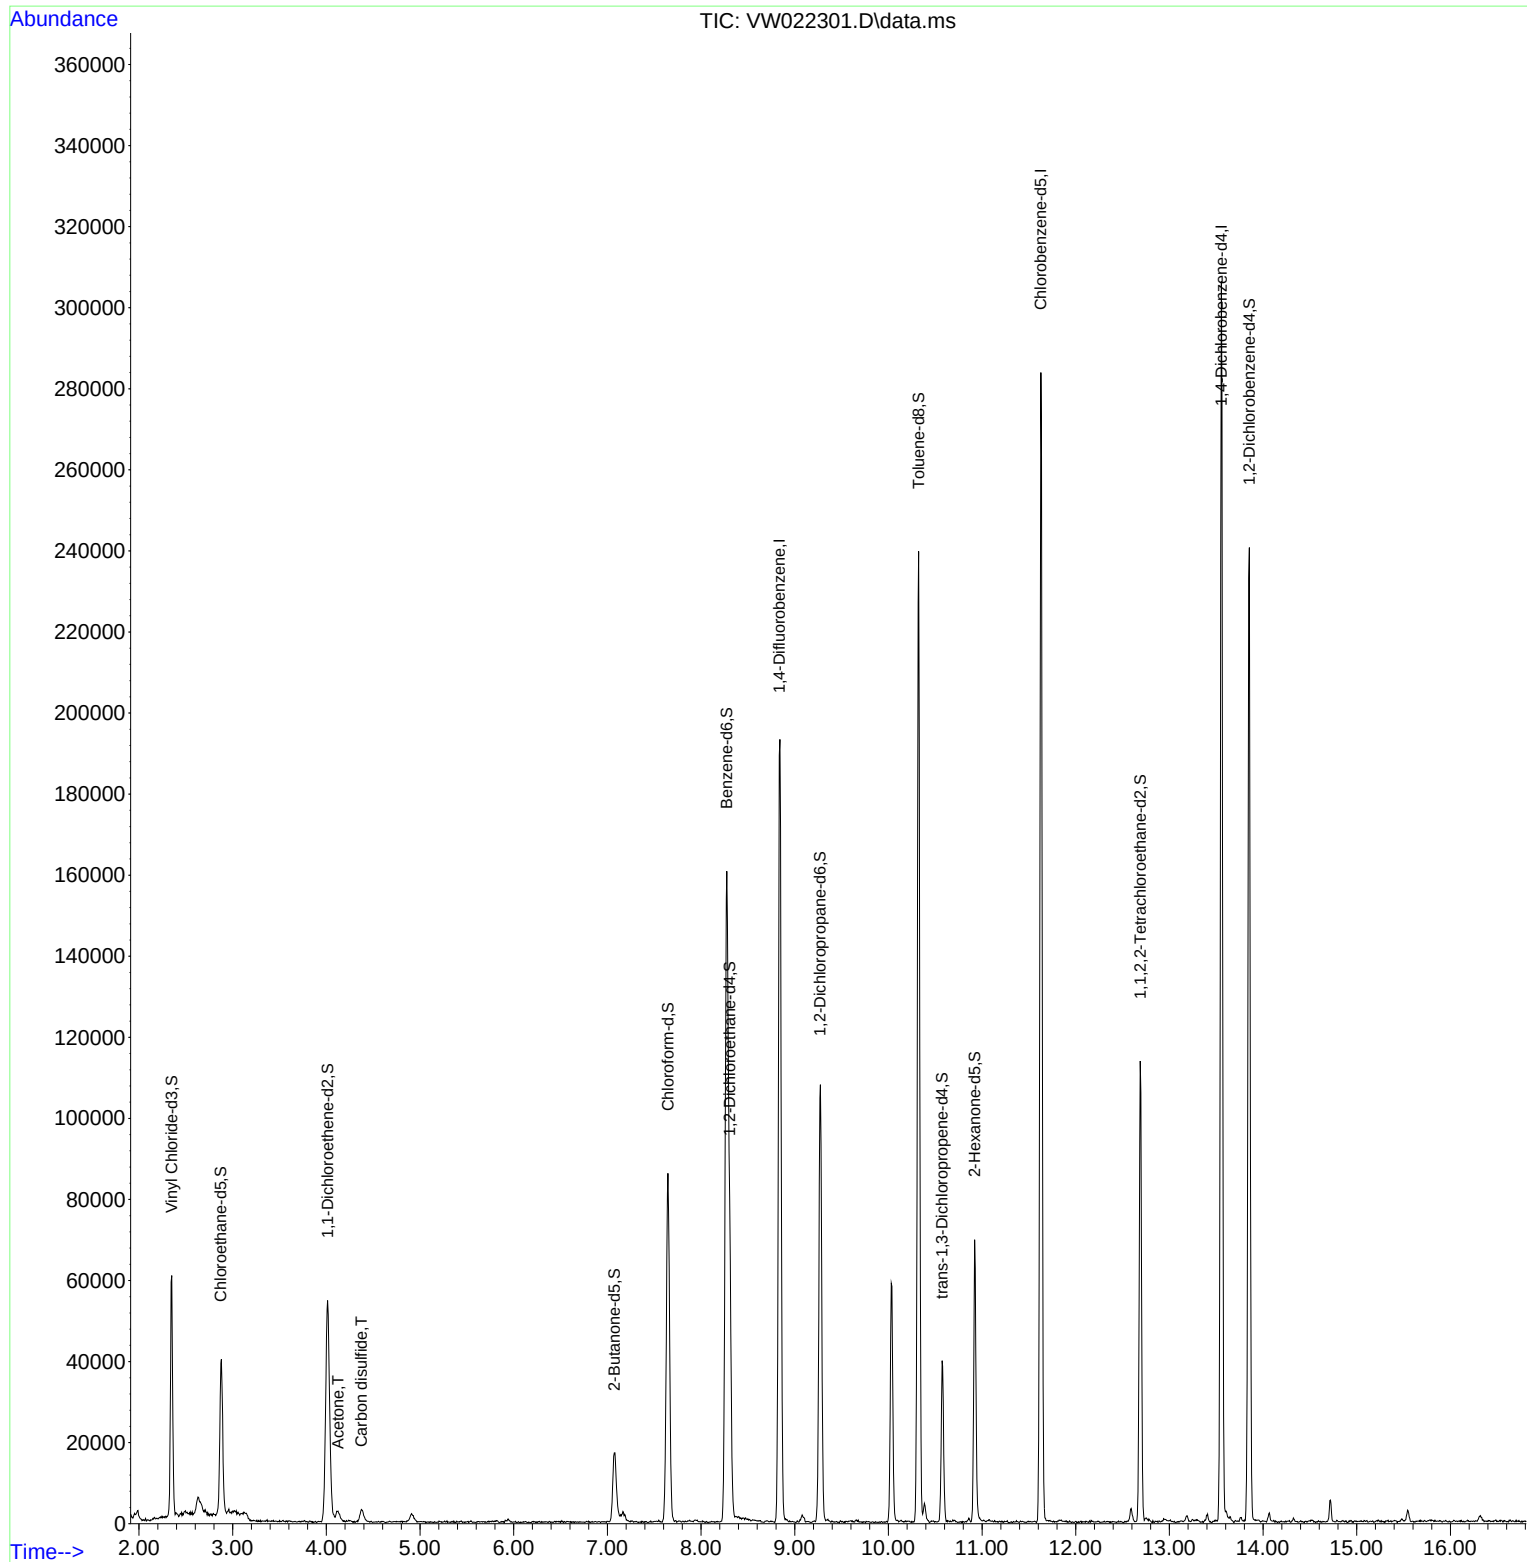


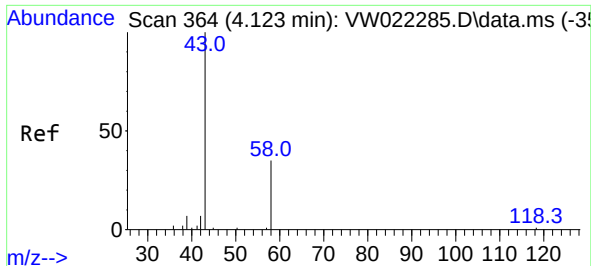

#13
Acetone
Concen: 13.545 ug/L
RT: 4.123 min Scan# 301
Delta R.T. -0.000 min
Lab File: VW022301.D
Acq: 11 Mar 2022 15:42

Instrument :
MSVOA_W
ClientSampleId :
DBRY3

Tgt Ion: 43 Resp: 4219
Ion Ratio Lower Upper
43 100
58 35.2 0.0 69.2

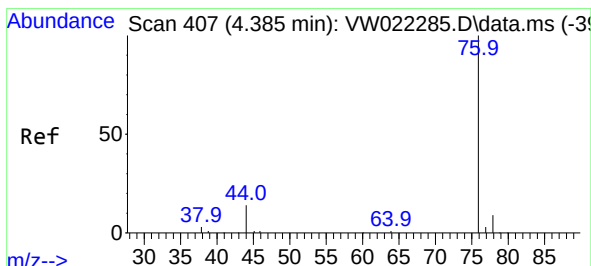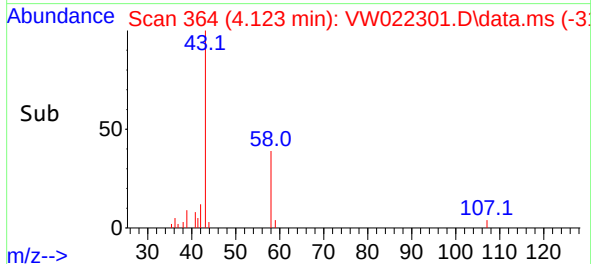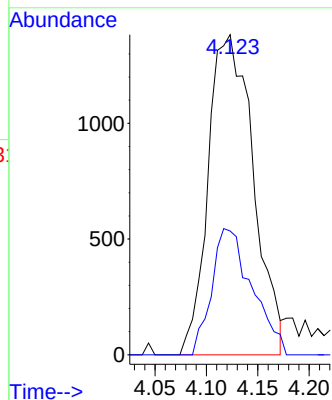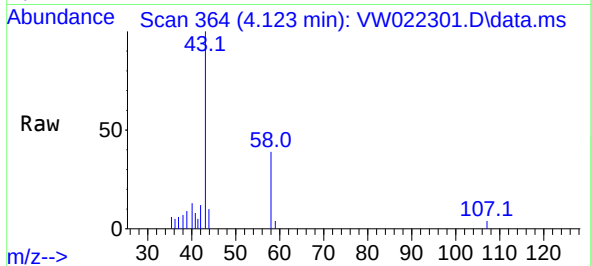

#14
Carbon disulfide
Concen: 1.422 ug/L
RT: 4.373 min Scan# 405
Delta R.T. -0.012 min
Lab File: VW022301.D
Acq: 11 Mar 2022 15:42

Tgt Ion: 76 Resp: 6621
Ion Ratio Lower Upper
76 100
78 10.8 7.8 11.8

