

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022306.D
 Acq On : 11 Mar 2022 17:44
 Operator : SY/VA
 Sample : N1819-21
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRZ1

Quant Time: Mar 11 21:06:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	167487	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	158901	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	76135	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	63643	29.133	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.520%
7) Chloroethane-d5	2.873	69	50642	29.463	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	117.840%
11) 1,1-Dichloroethene-d2	4.007	63	57334	17.138	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.560%
21) 2-Butanone-d5	7.080	46	22213	60.477	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.960%
24) Chloroform-d	7.647	84	95242	25.487	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.960%
26) 1,2-Dichloroethane-d4	8.305	65	51176	26.346	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.400%
32) Benzene-d6	8.274	84	180295	24.380	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.520%
36) 1,2-Dichloropropane-d6	9.268	67	52134	25.385	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.520%
41) Toluene-d8	10.323	98	171899	23.381	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.520%
43) trans-1,3-Dichloroprop...	10.573	79	21983	24.141	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.560%
47) 2-Hexanone-d5	10.920	63	18751	55.512	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.020%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	48323	26.811	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	65531	26.798	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.200%
Target Compounds					Qvalue	
13) Acetone	4.129	43	1823	6.077	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022306.D
Acq On : 11 Mar 2022 17:44
Operator : SY/VA
Sample : N1819-21
Misc : 5.61g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRZ1

Quant Time: Mar 11 21:06:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

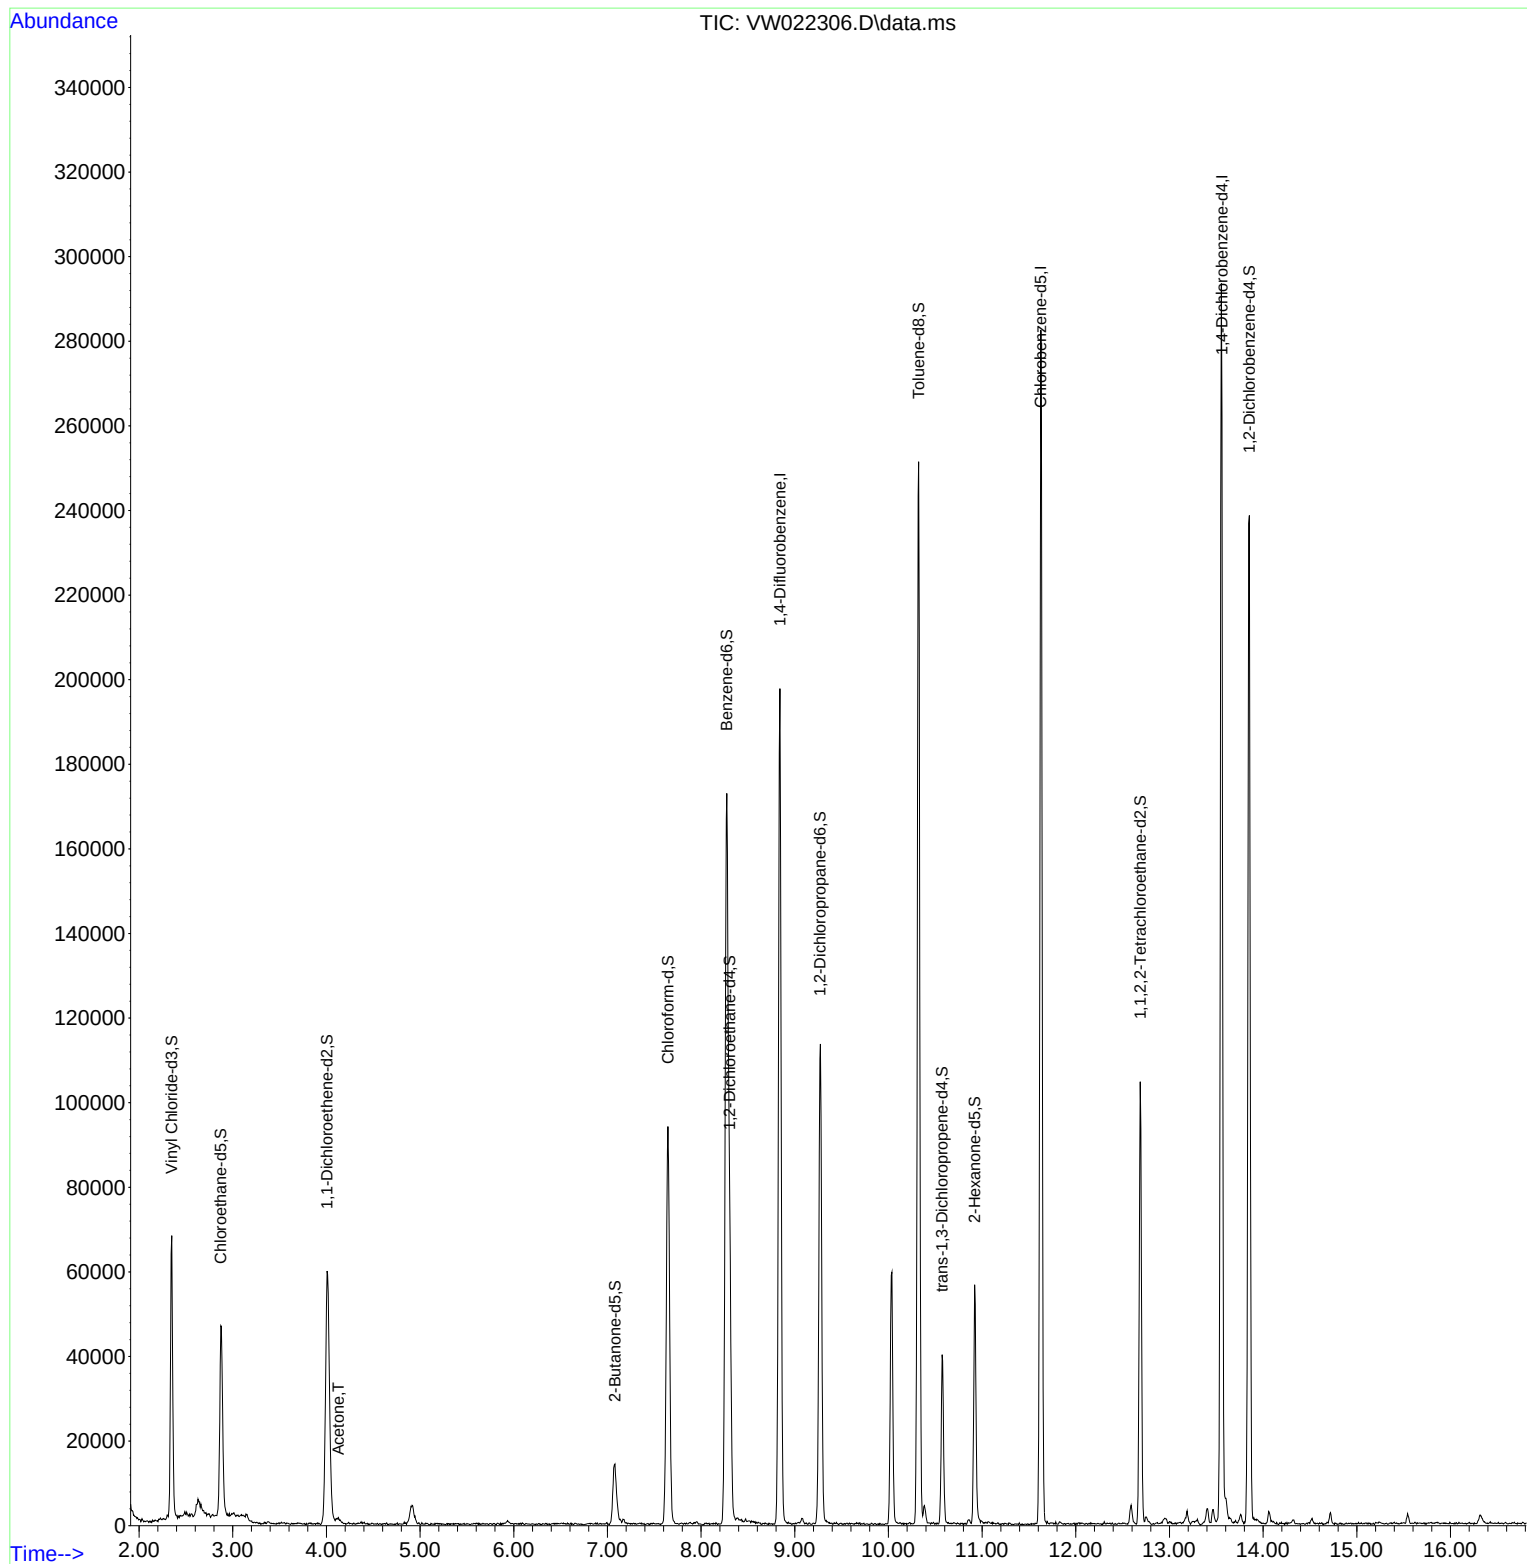

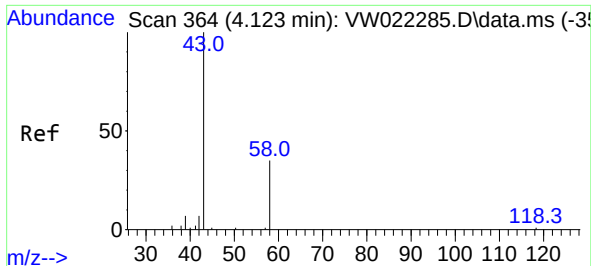

#13
 Acetone
 Concen: 6.077 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022306.D
 Acq: 11 Mar 2022 17:44

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRZ1

Tgt Ion: 43 Resp: 1823
 Ion Ratio Lower Upper
 43 100
 58 25.1 0.0 69.2

