

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
 Data File : VW022307.D
 Acq On : 11 Mar 2022 18:08
 Operator : SY/VA
 Sample : N1820-10
 Misc : 5.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG3

Quant Time: Mar 11 21:06:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 21:01:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	158044	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	155268	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78441	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	52290	25.366	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.480%
7) Chloroethane-d5	2.879	69	43381	26.747	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.000%
11) 1,1-Dichloroethene-d2	4.007	63	47906	15.176	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.720%
21) 2-Butanone-d5	7.074	46	22164	63.949	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.900%
24) Chloroform-d	7.647	84	80471	22.821	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.280%
26) 1,2-Dichloroethane-d4	8.305	65	46306	25.263	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.040%
32) Benzene-d6	8.268	84	150819	20.871	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.480%
36) 1,2-Dichloropropane-d6	9.268	67	44480	22.165	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.640%
41) Toluene-d8	10.323	98	143069	19.915	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.640%
43) trans-1,3-Dichloroprop...	10.573	79	19251	21.636	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.560%
47) 2-Hexanone-d5	10.920	63	18504	56.063	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.120%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	47547	26.997	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.000%
66) 1,2-Dichlorobenzene-d4	13.853	152	60335	23.948	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.800%
Target Compounds					Qvalue	
13) Acetone	4.123	43	987	3.487	ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022307.D
Acq On : 11 Mar 2022 18:08
Operator : SY/VA
Sample : N1820-10
Misc : 5.75g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG3


Quant Time: Mar 11 21:06:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 21:01:07 2022
Response via : Initial Calibration

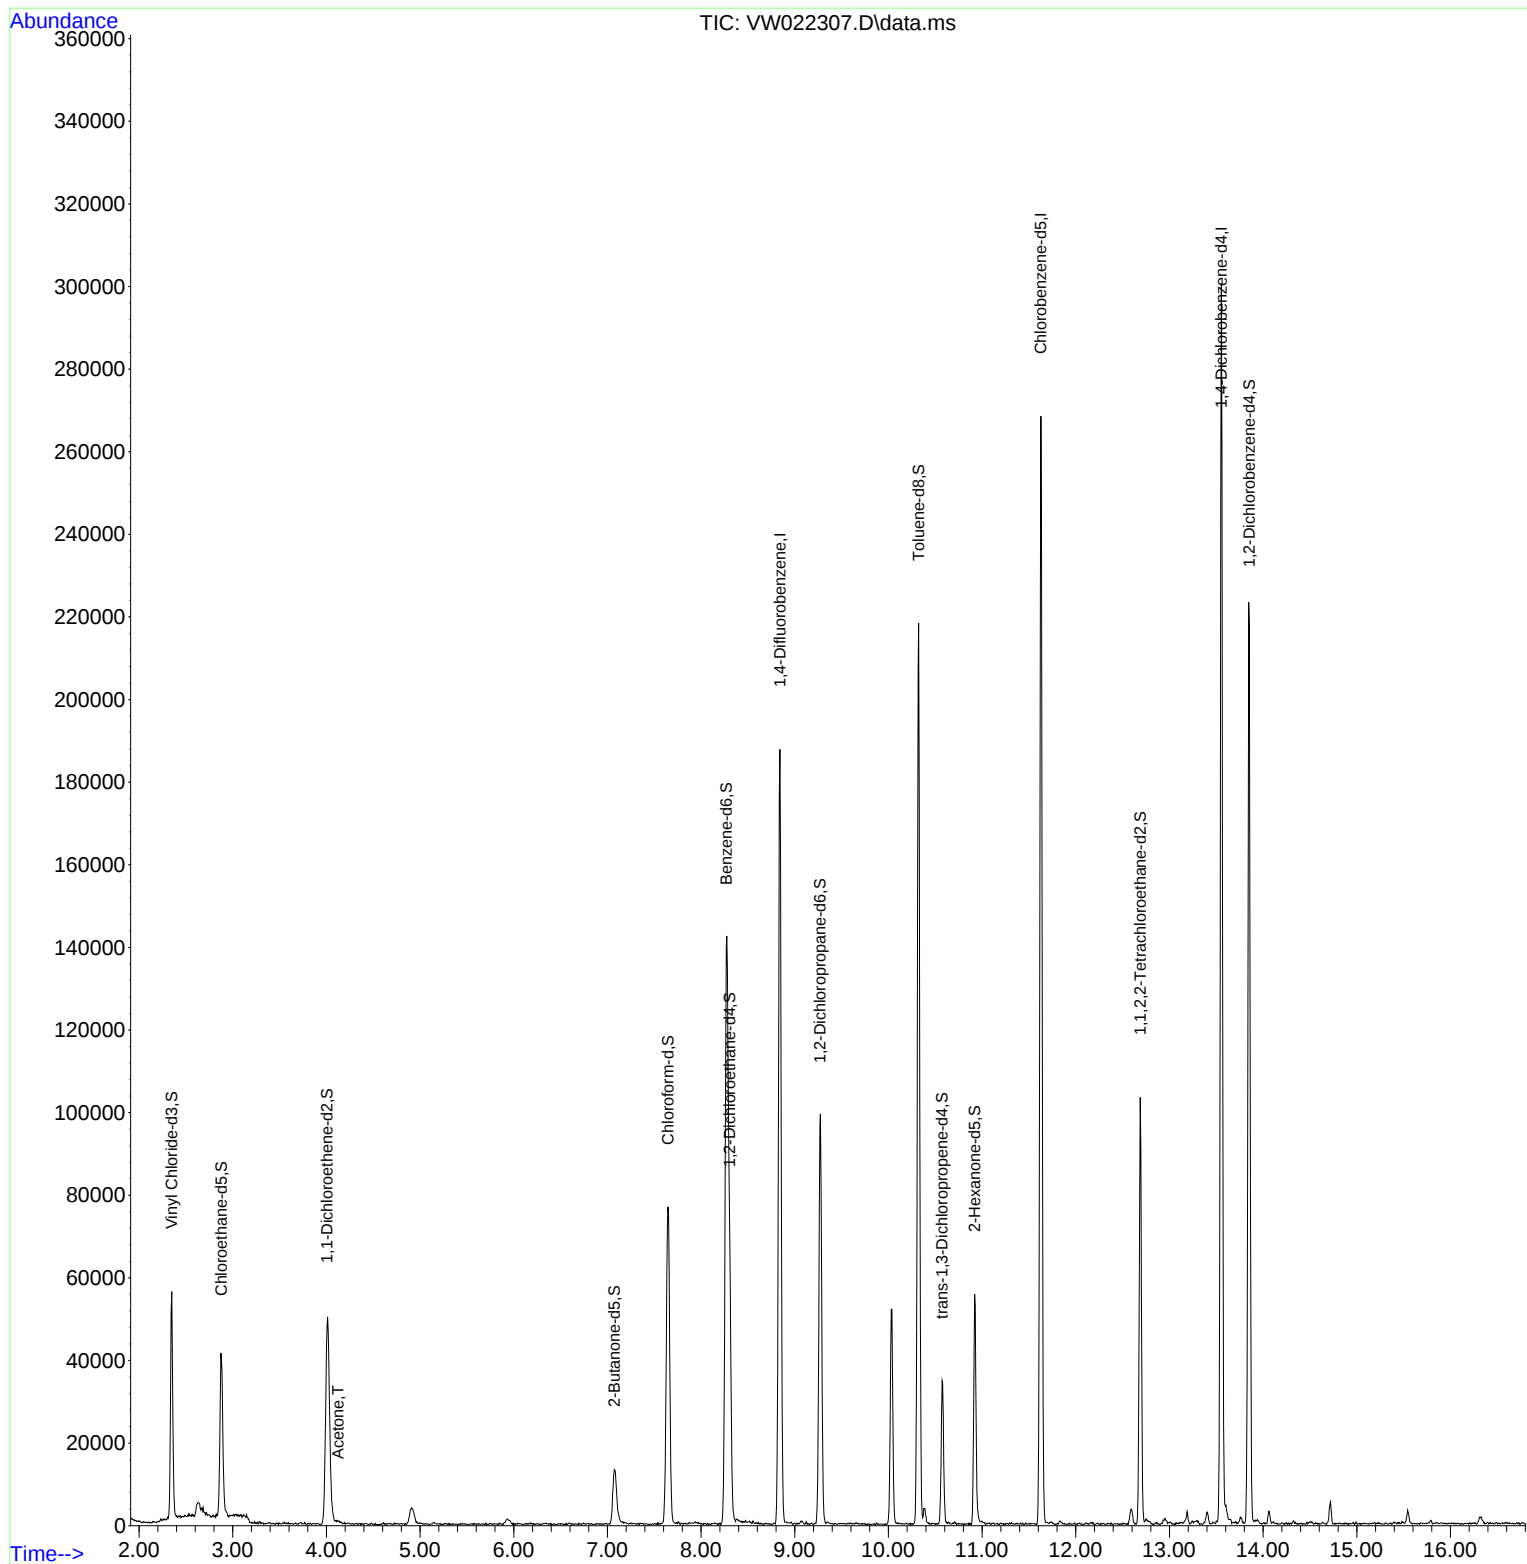

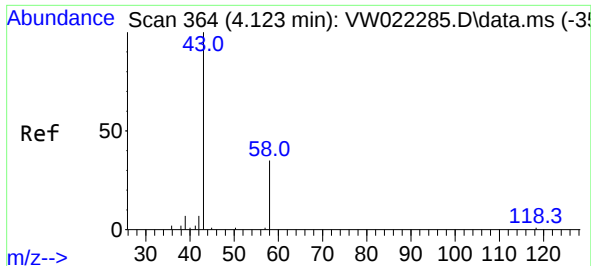

#13
 Acetone
 Concen: 3.487 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW022307.D
 Acq: 11 Mar 2022 18:08

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG3

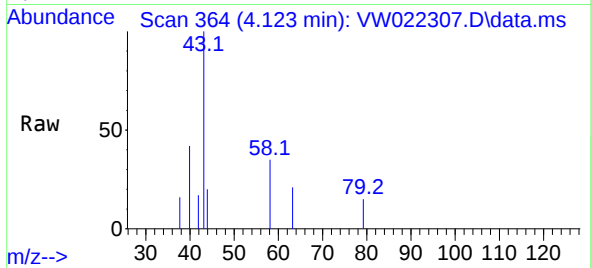

Tgt Ion: 43 Resp: 987

Ion	Ratio	Lower	Upper
43	100		
58	24.1	0.0	69.2

