


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031122\
Data File : VW022284.D
Acq On : 11 Mar 2022 07:46
Operator : SY/VA
Sample : BFB521
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB521

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Title : SFAM01.0
Last Update : Fri Mar 11 21:01:07 2022

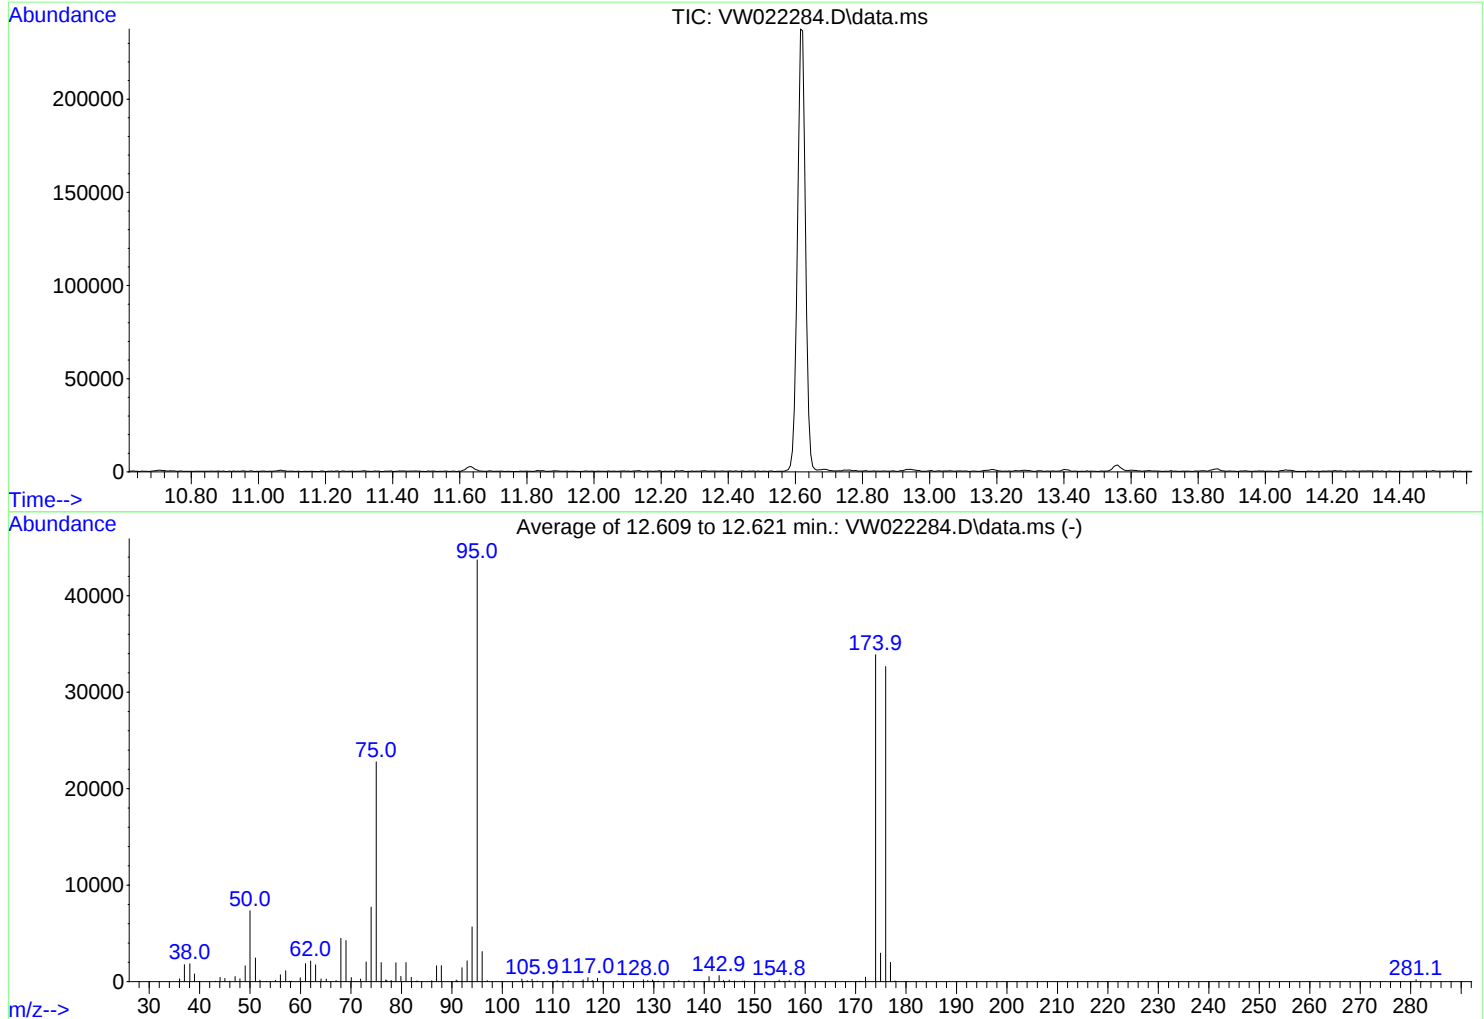

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	7342	PASS
75	95	30	80	52.1	22781	PASS
95	95	100	100	100.0	43717	PASS
96	95	5	9	7.1	3110	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.5	33883	PASS
175	174	5	9	8.7	2953	PASS
176	174	95	105	96.4	32653	PASS
177	176	5	10	6.1	1997	PASS

m/z	Abundance
39.90	164.0
43.80	77.0
44.90	54.0
57.10	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB521

m/z	Abundance
36.00	279.0
37.00	1388.0
38.00	1663.0
39.00	693.0
40.10	205.0
44.10	387.0
45.10	350.0
47.10	596.0
48.00	223.0
49.10	1412.0
50.00	6309.0
51.00	2215.0
51.90	174.0
53.30	54.0
55.00	103.0
56.00	549.0
57.00	1007.0
57.80	66.0
60.00	399.0
61.00	1673.0
62.00	1984.0
63.00	1537.0
64.00	199.0
65.10	193.0
68.00	3769.0
69.00	3469.0
70.00	381.0
72.00	172.0
73.00	1819.0
74.00	6780.0
75.00	19696.0
76.00	1689.0
76.90	232.0
78.00	176.0
78.90	1676.0
79.90	562.0
80.90	1584.0
82.00	364.0
82.90	91.0
86.00	89.0
87.00	1195.0
87.90	1609.0
91.10	215.0
92.00	1130.0
93.00	1827.0
94.00	4358.0
95.00	34176.0
96.00	2573.0
96.90	71.0
103.90	175.0
104.90	69.0
105.80	145.0
106.90	82.0
110.90	57.0
113.10	58.0
116.00	192.0
116.90	326.0
117.90	154.0
118.90	273.0
127.90	168.0
128.80	101.0
129.80	180.0
133.10	64.0
135.00	93.0
137.00	91.0
140.90	457.0
142.90	466.0
143.80	58.0
145.00	126.0
146.00	70.0
148.00	89.0
154.80	92.0
157.00	59.0
160.80	55.0
170.80	102.0
171.90	440.0
173.90	23696.0
174.90	1881.0
176.00	22944.0
176.90	1624.0
281.00	205.0
282.10	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB521

m/z	Abundance
36.10	297.0
37.00	1899.0
38.10	1962.0
39.00	806.0
39.90	250.0
43.20	83.0
44.00	439.0
45.00	489.0
46.00	77.0
47.00	516.0
48.00	357.0
49.00	1755.0
50.00	7749.0
51.00	2675.0
52.00	92.0
53.30	60.0
55.10	148.0
56.00	732.0
57.00	1377.0
57.80	68.0
58.20	79.0
59.90	481.0
61.00	2001.0
62.00	2195.0
63.00	1715.0
64.00	230.0
65.10	272.0
67.00	217.0
68.00	5019.0
69.00	4859.0
70.10	512.0
71.80	280.0
73.00	2379.0
74.00	8502.0
75.00	25008.0
76.00	2317.0
76.90	326.0
77.90	201.0
78.90	2151.0
79.90	567.0
80.90	2238.0
81.90	454.0
83.10	99.0
86.00	108.0
87.00	2058.0
87.90	1678.0
90.80	259.0
92.00	1558.0
93.00	2367.0
94.00	6420.0
95.00	49096.0
96.00	3667.0
97.00	148.0
103.80	298.0
104.90	94.0
105.90	273.0
106.90	77.0
110.90	108.0
113.10	117.0
115.90	189.0
117.00	438.0
117.70	201.0
118.80	371.0
128.00	212.0
128.70	118.0
129.70	139.0
130.00	156.0
130.70	108.0
134.90	133.0
136.80	112.0
140.90	571.0
142.90	711.0
143.80	174.0
144.90	260.0
146.00	121.0
147.70	93.0
148.00	120.0
149.90	80.0
154.90	171.0
155.80	60.0
156.80	185.0
158.80	98.0
170.10	74.0
172.00	526.0
174.00	37424.0
175.00	3435.0
176.00	36224.0
177.00	2496.0
177.80	79.0
281.10	286.0
282.10	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB521

m/z	Abundance
36.10	317.0
37.00	1994.0
38.00	1951.0
39.00	891.0
40.00	130.0
43.00	73.0
44.00	513.0
45.00	337.0
46.00	82.0
47.00	468.0
48.00	300.0
49.00	1762.0
50.00	7968.0
51.10	2489.0
52.00	204.0
55.00	180.0
56.00	839.0
57.10	1244.0
58.20	68.0
60.00	309.0
61.00	1948.0
62.00	2236.0
63.00	1967.0
64.10	411.0
64.90	161.0
65.20	165.0
67.10	155.0
68.00	4721.0
69.00	4454.0
70.00	398.0
70.90	72.0
71.90	321.0
73.00	1929.0
74.00	7920.0
75.00	23640.0
76.00	1942.0
77.10	398.0
78.90	2037.0
79.90	532.0
80.90	2106.0
81.90	535.0
83.10	138.0
86.00	87.0
86.90	1666.0
87.90	1669.0
90.90	233.0
92.00	1641.0
93.00	2295.0
94.00	6254.0
95.00	47880.0
96.00	3091.0
97.10	144.0
103.90	319.0
105.00	115.0
106.00	320.0
106.90	57.0
110.80	127.0
112.90	84.0
115.70	149.0
116.10	173.0
116.90	485.0
118.00	218.0
118.90	407.0
123.80	51.0
126.70	52.0
127.90	186.0
128.90	124.0
129.80	199.0
130.90	140.0
135.00	90.0
137.10	158.0
141.00	567.0
141.90	73.0
143.00	723.0
143.80	103.0
145.00	109.0
147.60	102.0
150.00	54.0
152.10	58.0
154.90	227.0
155.70	62.0
156.90	124.0
158.80	106.0
160.90	58.0
171.00	105.0
171.90	435.0
173.90	40528.0
174.90	3542.0
175.90	38792.0
176.80	1870.0
177.80	113.0
281.00	139.0

Instrument :
MSVOA_W
ClientSampleId :
BFB521