
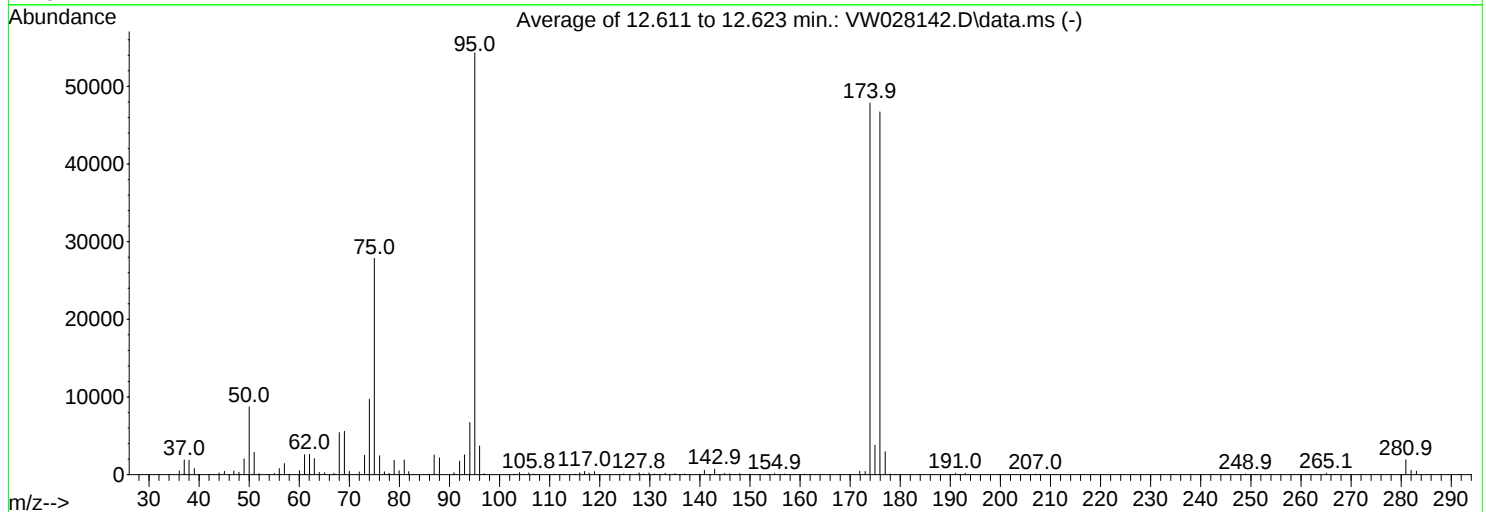


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031124\
Data File : VW028142.D
Acq On : 11 Mar 2024 08:40
Operator : SY/MD
Sample : BFB450
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB450

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Title : SFAM01.0
Last Update : Tue Mar 12 01:08:51 2024

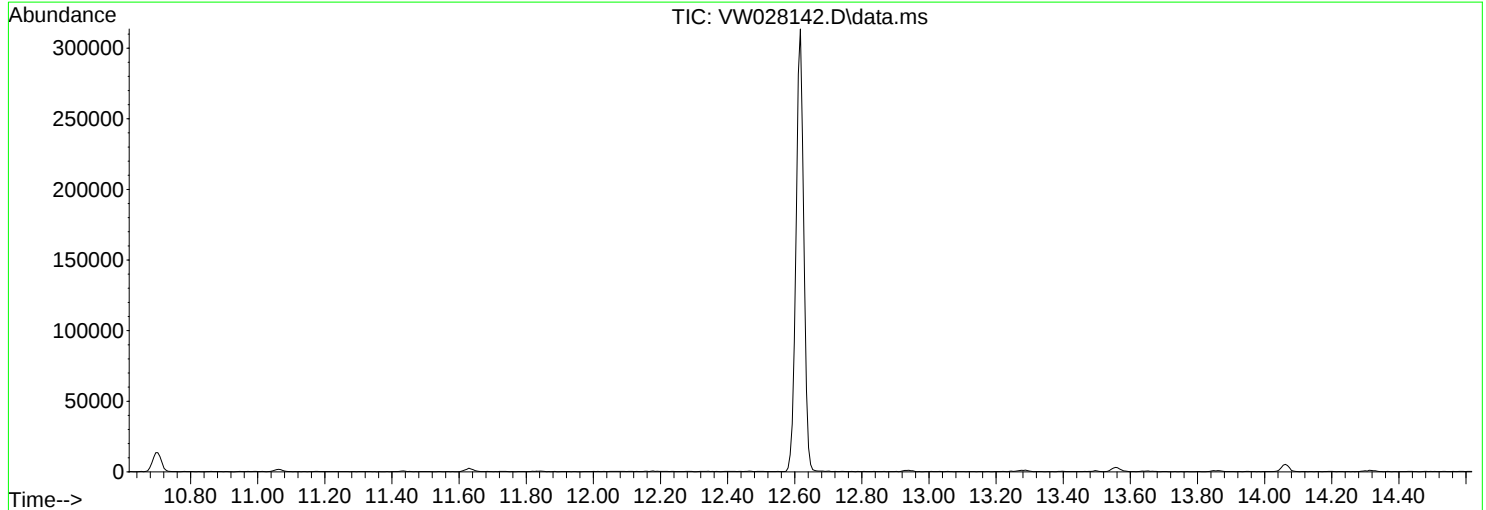

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	8742	PASS
75	95	30	80	51.3	27859	PASS
95	95	100	100	100.0	54320	PASS
96	95	5	9	6.8	3680	PASS
173	174	0.00	2	0.9	407	PASS
174	95	50	120	88.1	47845	PASS
175	174	5	9	7.9	3797	PASS
176	174	95	101	97.6	46717	PASS
177	176	5	9	6.3	2966	PASS

m/z	Abundance
35.80	97.0
40.00	71.0
44.00	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.10	443.0
37.00	2068.0
38.00	1822.0
39.00	903.0
40.10	142.0
42.90	69.0
44.10	412.0
45.00	452.0
46.00	53.0
47.00	612.0
48.00	302.0
49.00	2221.0
50.00	9610.0
51.00	3175.0
52.00	179.0
55.00	195.0
56.00	953.0
57.10	1449.0
58.00	81.0
60.00	610.0
61.10	2979.0
62.10	2882.0
63.00	2302.0
64.00	312.0
65.10	236.0
66.90	132.0
68.00	5688.0
69.00	5942.0
70.00	460.0
72.00	340.0
73.10	2776.0
74.00	10028.0
75.00	28904.0
76.10	2721.0
77.00	405.0
77.90	223.0
78.90	2040.0
80.00	532.0
81.00	2059.0
81.90	392.0
82.90	54.0
85.80	79.0
87.00	2731.0
88.00	2210.0
90.90	195.0
92.00	1681.0
93.00	2788.0
94.00	6436.0
95.00	57152.0
96.00	3921.0
96.90	193.0
102.90	145.0
103.90	315.0
105.80	143.0
106.80	76.0
110.00	55.0
110.80	98.0
112.00	66.0
115.00	57.0
116.00	262.0
116.90	449.0
117.80	284.0
118.90	361.0
124.80	132.0
127.80	240.0
129.00	92.0
129.90	274.0
130.90	98.0
133.10	430.0
133.90	101.0
135.00	174.0
136.90	88.0
140.90	491.0
142.10	81.0
143.00	805.0
144.90	149.0
145.90	75.0
146.90	62.0
147.90	186.0
149.90	94.0
153.70	64.0
154.90	166.0
156.90	96.0
160.90	61.0
163.10	57.0
171.90	512.0
173.90	42608.0
175.00	3987.0
176.00	43960.0
177.00	2949.0
177.90	87.0
179.10	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

191.00	291.0
191.90	71.0
193.00	336.0
204.80	55.0
207.00	163.0
207.90	73.0
248.90	195.0
250.90	100.0
265.00	345.0
266.80	59.0
280.90	2861.0
282.00	972.0
283.10	879.0
284.10	153.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.00	601.0
37.10	2148.0
38.00	2260.0
39.10	886.0
40.10	115.0
44.00	279.0
45.00	429.0
46.00	52.0
46.90	468.0
48.00	387.0
49.00	2334.0
50.00	9587.0
51.00	3163.0
52.00	154.0
55.10	126.0
56.00	681.0
57.00	1613.0
58.10	75.0
60.10	469.0
61.00	2758.0
62.00	2944.0
63.00	2427.0
64.00	324.0
65.00	283.0
67.00	217.0
68.00	6060.0
69.00	6341.0
70.00	542.0
72.00	531.0
73.00	2781.0
74.00	10693.0
75.00	31416.0
76.10	2623.0
77.00	399.0
78.10	242.0
79.00	1927.0
80.00	530.0
80.90	2101.0
81.80	470.0
85.80	92.0
86.90	2816.0
88.00	2358.0
90.90	348.0
92.00	1982.0
93.00	2661.0
94.10	7855.0
95.00	60424.0
96.00	4097.0
96.90	117.0
103.00	68.0
104.00	287.0
104.80	52.0
105.90	313.0
106.90	85.0
109.90	53.0
110.90	70.0
112.90	108.0
114.80	83.0
115.20	77.0
116.00	281.0
116.90	421.0
117.90	152.0
118.90	410.0
124.80	92.0
127.90	287.0
128.70	89.0
129.80	197.0
131.00	63.0
132.90	155.0
133.70	55.0
135.00	178.0
137.00	131.0
140.10	76.0
140.90	760.0
141.90	55.0
143.00	853.0
143.80	50.0
145.00	218.0
145.90	136.0
147.90	99.0
148.80	60.0
149.90	94.0
154.90	175.0
157.00	120.0
158.80	61.0
160.90	113.0
171.90	522.0
173.00	771.0
174.00	56504.0
174.90	4161.0
176.00	53224.0
177.00	3486.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

178.00	148.0
191.00	209.0
192.90	198.0
204.80	69.0
207.00	111.0
249.00	117.0
265.10	127.0
266.10	61.0
281.00	2325.0
282.00	466.0
283.00	305.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.00	396.0
37.10	1499.0
38.00	1514.0
39.00	577.0
39.90	126.0
44.00	275.0
45.10	393.0
47.00	368.0
47.90	232.0
49.00	1567.0
50.00	7028.0
51.00	2322.0
52.00	112.0
55.00	119.0
56.00	691.0
57.00	1204.0
60.00	439.0
61.00	2023.0
62.00	2041.0
63.00	1466.0
64.00	210.0
65.10	252.0
66.90	128.0
68.00	4491.0
69.00	4473.0
70.00	271.0
72.00	207.0
73.00	1933.0
74.00	8408.0
75.00	23256.0
76.00	1948.0
77.00	293.0
77.90	190.0
79.00	1574.0
79.90	496.0
80.90	1532.0
81.90	285.0
87.00	2085.0
88.00	1918.0
90.90	231.0
92.00	1563.0
93.00	2219.0
94.00	5833.0
95.10	45384.0
96.00	3021.0
96.90	66.0
103.90	222.0
104.90	59.0
105.90	254.0
106.80	72.0
115.10	75.0
115.90	178.0
117.00	384.0
117.90	210.0
119.00	414.0
124.80	88.0
127.90	136.0
128.80	155.0
129.90	192.0
130.90	62.0
134.90	113.0
136.90	98.0
140.90	421.0
142.80	496.0
144.90	108.0
145.90	89.0
147.90	71.0
149.90	74.0
154.80	107.0
156.90	78.0
160.90	64.0
171.80	338.0
173.00	449.0
174.00	44424.0
175.00	3242.0
175.90	42968.0
177.00	2463.0
178.00	85.0
191.00	57.0
265.10	86.0
281.10	587.0
281.90	291.0
283.10	168.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450