


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW031219\
 Data File : VW009133.D
 Acq On : 13 Mar 2019 02:19
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W030719S.M
 Title : SW846 8260
 Last Update : Fri Mar 08 05:22:30 2019

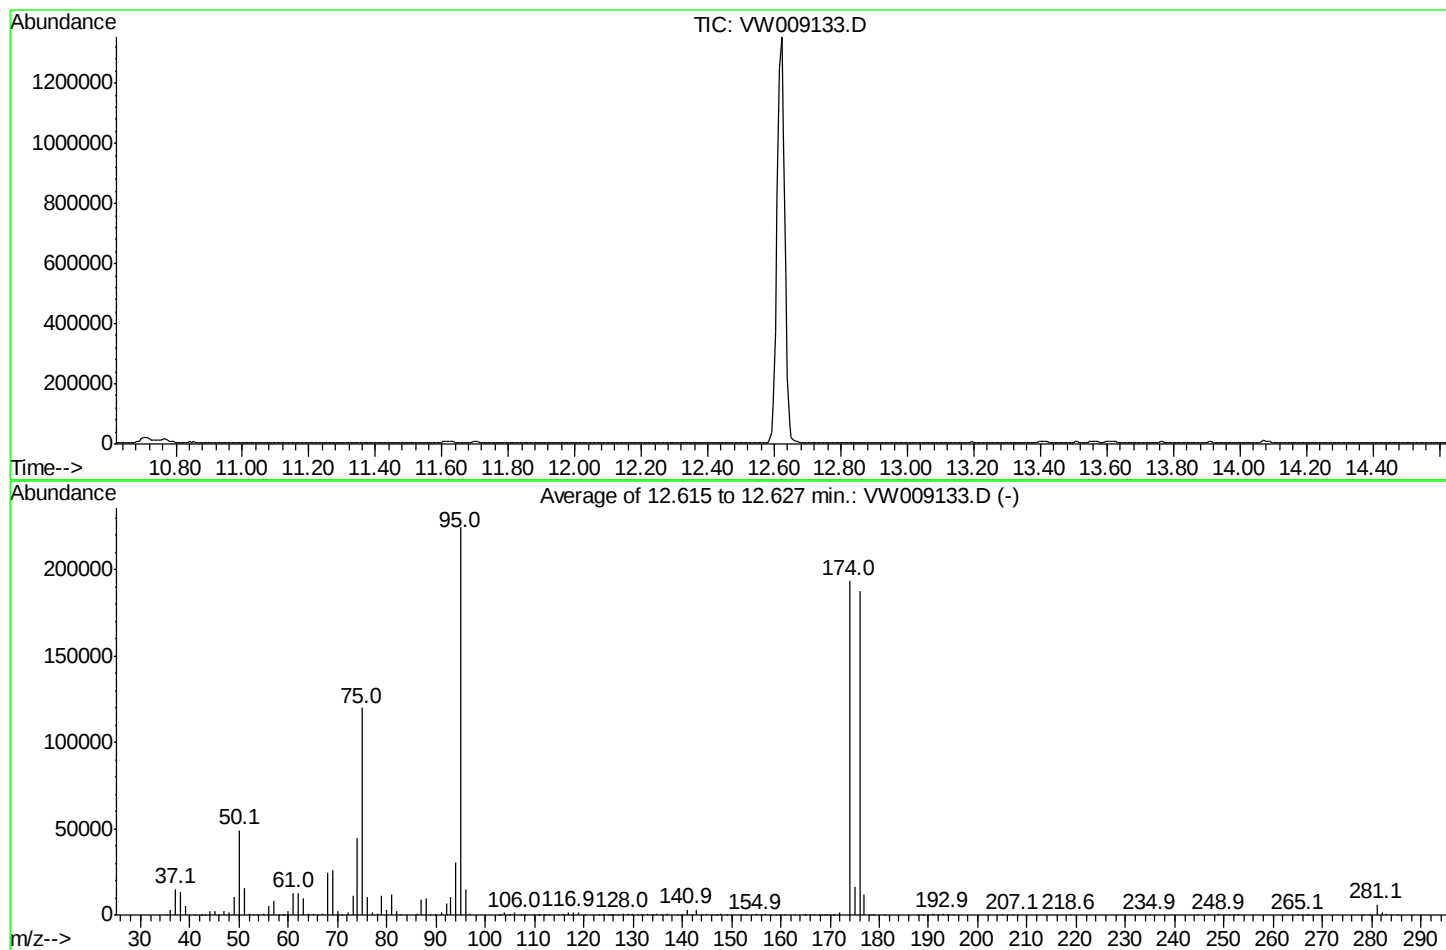

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	49288	PASS
75	95	30	60	53.4	119805	PASS
95	95	100	100	100.0	224384	PASS
96	95	5	9	6.5	14511	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.2	193450	PASS
175	174	5	9	8.3	15965	PASS
176	174	95	101	96.8	187200	PASS
177	176	5	9	6.4	11986	PASS